

IBM TotalStorage Storage Switch



2006 Model L10 Installation and User's Guide

Read Before Using

This product contains software that is licensed under written license agreements. Your use of such software is subject to the license agreements under which they are provided.

IBM TotalStorage Storage Switch



2006 Model L10 Installation and User's Guide

Note:

Before using this information and the product it supports, read the information in the *Safety Information* document.

First Edition (August 2004)

Form Number GC26-7651-00

Part Number 26K7913

The following paragraph does not apply to any country (or region) where such provisions are inconsistent with local law.

INTERNATIONAL BUSINESS MACHINES CORPORATION PROVIDES THIS PUBLICATIONS "AS IS" WITHOUT WARRANTY OF ANY KIND, EITHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. Some states (or regions) do not allow disclaimer of express or implied warranties in certain transactions; therefore, this statement may not apply to you.

Order publications through your IBM representative or the IBM branch office serving your locality.

© Copyright International Business Machines Corporation 2004. All rights reserved.

US Government Users Restricted Rights – Use, duplication or disclosure restricted by GSA ADP Schedule Contract with IBM Corp.

© 2004 Emulex Corporation. All rights reserved.

Part Number 00041459-001 Rev. A

Emulex and Vixel are registered trademarks, and InSpeed and FibreSpy are trademarks, of Emulex Corporation. All other brand or product names referenced herein are trademarks or registered trademarks of their respective companies or organizations.

Contents

Contents	.iii
Figures	vii
Tables	.ix
Safety and environmental notices	.xi
Safety notices and labels	.xi
Danger notices	.xi
Labels	.xiii
Caution notices	.xiii
Attention notices	.xiv
Safety inspections, installations, and service	.xiv
Laser safety	.xiv
Usage restrictions	.xiv
Environmental notices and statements	.xv
Fire suppression systems	.xv
Product recycling	.xv
Product disposal	.xv
About this document	xvii
Model L10 library	xvii
Web sites	xvii
Getting software updates	xviii
Getting help	xviii
Online	xviii
Telephone	xviii
How to send your comments	xviii
Chapter 1. Introduction	1
Features	2
InSpeed™ technology	3
Chapter 2. Switch installation	5
Installation preparation	5
Switch installation	6
Rack installation	6
Desktop installation	6
Switch LEDs	7
Ethernet LEDs	7
System LEDs	8
Port LEDs	9
Serial port	9
SFP compatibility	10
Installing an SFP	10
Removing an SFP	10

Attaching a device to the switch	10
Booting the switch and SAN	11
Chapter 3. Switch management	13
Getting started	13
Configuring the network interface	13
Connecting to the Web Manager	15
Web Manager overview	15
Initial switch setup	17
Managing the switch	19
Logging in to the switch	20
Configuring the switch settings	20
Opening a telnet session	25
Adjusting the switch thresholds	26
Configuring the port Smart Settings	27
Managing firmware and configuration files	35
One-step zoning	37
Cascading switches	43
Automatic trunking	45
Load balancing	46
Monitoring the switch	49
Viewing switch status	49
Viewing the Event Log	51
Viewing port information	52
Viewing port utilization	52
Viewing port diagnostics	53
Viewing ordered sets	55
Chapter 4. Technical reference	57
Troubleshooting device connections	57
Troubleshooting management connections	58
Port bypass conditions and recovery	58
Default Smart Setting attributes	59
Appendix A: Specifications	61
Switch specifications	61
Operating conditions	61
Appendix B: CLI quick reference	63
Connecting to the CLI	63
Logging in and out	63
Using the CLI	64
Frequent switch configuration tasks	64
CLI commands	65
Appendix C: Event messages	67
Appendix D: AL_PA cross references	69
Notices	71

Trademarks	71
Electronic emission notices	72
Federal Communications Commission (FCC) Class A Statement	72
Industry Canada Class A Emission Compliance Statement	72
Avis de conformité à la réglementation d'Industrie Canada	72
European Union (EU) Electromagnetic Compatibility Directive	72
Germany Electromagnetic Compatibility Directive.	73
Japan VCCI Class A ITE Electronic Emission Statement	73
Glossary	75
Index	77

Figures

1. Switch view depicting Ethernet, port, and system LEDs	7
2. Ethernet LEDs	7
3. System LEDs	8
4. Port LEDs	9
5. Switch view depicting DB-9 serial port	9
6. Web Manager interface	15
7. Switch Login page	20
8. Switch Configuration page	21
9. Switch SNMP Trap Configuration page	23
10. Switch Date & Time page	24
11. Switch Password page	25
12. Switch Thresholds page	26
13. Port Smart Settings page	27
14. Port Smart Settings page (all options displayed)	27
15. Switch Files page	35
16. One-Step Zoning page	37
17. Devices in a single zone	39
18. Single switch zoning configuration	39
19. Devices in multiple zones	40
20. Ports in multiple zones on the One-Step Zoning page	40
21. Devices in multiple zones across multiple switches	41
22. Zones coordinated on multiple switches	41
23. Hard Zoning configuration	43
24. String cascade configuration example	44
25. Tree cascade configuration example	44
26. Automatic Trunking example	45
27. Advanced Functions: Automatic Trunking page	46
28. Load balancing across multiple cascade ports	46
29. Advanced Functions: Load Balancing page	47
30. Switch Information page	49
31. Switch Event Log page	51
32. Port Information page	52
33. Port Utilization page	53
34. Advanced Functions: Port Diagnostics page	53
35. Advanced Functions: Ordered Sets page	55

Tables

1. Ethernet LED descriptions	7
2. System LED descriptions	8
3. Port LED descriptions	9
4. Web Manager command buttons	16
5. Frequent switch configuration tasks	19
6. Switch identification settings	21
7. Network location settings	22
8. Software and hardware version information	22
9. Switch speed settings	23
10. SNMP trap settings	24
11. Switch threshold settings	26
12. Port information settings	31
13. Pre-insertion testing settings	31
14. Change notification settings	32
15. Port recovery settings	33
16. Diagnostic settings	34
17. Zone color status	37
18. Switch status information	49
19. Port number colors and indications	50
20. Port utilization colors and indications	50
21. Port information settings and descriptions	52
22. Port utilization values and descriptions	53
23. Port statistics and descriptions	54
24. Ordered sets and descriptions	56
25. Device connection issues and recommended actions	57
26. Management connection issues and recommended actions	58
27. Port bypass conditions and recovery	58
28. Default Smart Setting attributes	59
29. Switch specifications	61
30. Operating conditions	61
31. Switch configuration tasks	64
32. CLI command quick reference	65
33. Event message severity levels	67
34. Event message information	67
35. AL_PA cross references	69
36. Glossary terms	75

Safety and environmental notices

This section contains information about:

- “Safety notices and labels”
- “Safety inspections, installations, and service”
- “Environmental notices and statements”

Safety notices and labels

When using this product, observe the danger, caution, and attention notices contained in this guide. The notices are accompanied by symbols that represent the severity of the safety condition.

Danger notices

A danger notice calls attention to a situation that is potentially lethal or extremely hazardous to people. A lightning bolt symbol accompanies a danger notice to represent a dangerous electrical condition. A sample danger notice follows:



DANGER

An electrical outlet that is not correctly wired could place hazardous voltage on metal parts of the system or the devices that attach to the system. It is the responsibility of the customer to ensure that the outlet is correctly wired and grounded to prevent an electrical shock. (D004)

The danger notice below provides instructions on how to avoid shock hazards when servicing equipment. Unless instructed otherwise, follow the procedures in the danger notice below:



DANGER

Electrical voltage and current from power, telephone, and communication cables are hazardous.

To avoid a shock hazard:

- Do not connect or disconnect any cables or perform installation, maintenance, or reconfiguration of this product during an electrical storm.
- Connect all power cords to a properly wired and grounded electrical outlet. Ensure outlet supplies proper voltage and phase rotation according to the system rating plate.
- Connect any equipment that will be attached to this product to properly wired outlets.
- When possible, use one hand only to connect or disconnect signal cables.
- Never turn on any equipment when there is evidence of fire, water, or structural damage.
- Disconnect the attached power cords, telecommunications, systems, networks, and modems before you open the device covers, unless instructed otherwise in the installation and configuration procedures.
- Connect and disconnect cables as described below when installing, moving, or opening covers on this product or attached devices.

To Disconnect:

1. Turn everything OFF (unless instructed otherwise).
2. Remove power cords from the outlet.
3. Remove signal cables from connectors.
4. Remove all cables from devices.

To Connect:


1. Turn everything OFF (unless instructed otherwise).
2. Attach all cables to devices.
3. Attach signal cables to connectors.
4. Attach power cords to outlet.
5. Turn device ON.

(D005)

Labels

As an added precaution, safety labels are often installed directly on products or product components to warn of potential hazards.

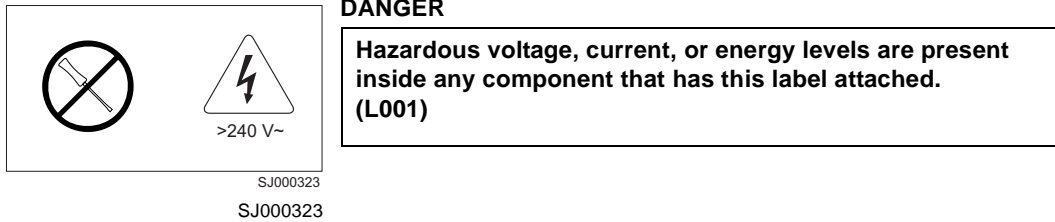


The actual product safety labels may differ from the sample safety label:



Do not service, there are no serviceable parts.

Caution notices

A caution notice calls attention to a situation that is potentially hazardous to people because of some existing condition. A caution notice can be accompanied by different symbols, as in the examples below:

If the symbol is...	It means...
	A hazardous electrical condition with less severity than electrical danger.
	A generally hazardous condition not represented by other safety symbols.
	A hazardous condition due to the use of a laser in the product. Laser symbols are always accompanied by the classification of the laser as defined by the U.S. Department of Health and Human Services (for example, Class I, Class II, and so forth).

Sample caution notices:



CAUTION

This product is equipped with a 3-wire (two conductors and ground) power cable and plug. Use this power cable with a properly grounded electrical outlet to avoid electrical shock. (C018)



Class I

CAUTION

This product contains a Class 1M laser. Do not view directly with optical instruments. (C028)

Attention notices

An attention notice indicates the possibility of damage to a program, device, or system, or to data. An exclamation point symbol may accompany an attention notice, but is not required. A sample attention notice follows:



Attention: Do not over-tighten the screws, this can damage the backplane.

Safety inspections, installations, and service

Laser safety

This equipment contains Class 1 laser products, and complies with FDA radiation Performance Standards, 21 CFR Subchapter J and the international laser safety standard IEC 825-2.



Class I

CAUTION

This product contains a Class 1M laser. Do not view directly with optical instruments. (C028)

Attention: In the United States, use only SFP or GBIC optical transceivers that comply with the FDA radiation performance standards, 21 CFR Subchapter J. Internationally, use only SFP or GBIC optical transceivers that comply with IEC standard 825-1. Optical products that do not comply with these standards may produce light that is hazardous to the eyes.

Usage restrictions

The optical ports of the modules must be terminated with an optical connector or with a dust plug.

Environmental notices and statements

Fire suppression systems

A fire suppression system is the responsibility of the customer. The customer's own insurance underwriter, local fire marshal, or a local building inspector, or both, should be consulted in selecting a fire suppression system that provides the correct level of coverage and protection. IBM designs and manufactures equipment to internal and external standards that require certain environments for reliable operation. Because IBM does not test any equipment for compatibility with fire suppression systems, IBM does not make compatibility claims of any kind nor does IBM provide recommendations on fire suppression systems.

Product recycling

This unit contains recyclable materials. These materials should be recycled where processing sites are available and according to local regulations. In some areas, IBM provides a product take-back program that ensures proper handling of the product. Contact your IBM representative for more information.

Product disposal

This unit might contain batteries. Remove and discard these batteries, or recycle them, according to local regulations.

About this document

This guide provides you with the necessary information to install and manage the IBM TotalStorage Storage Switch 2006 Model L10 for use in Fibre Channel applications in typical entry-level Storage Area Networks (SANs).

Throughout the rest of this document, the IBM TotalStorage® Storage Switch 2006 Model L10 is referred to as the Model L10, the L10, or simply the switch.

The sections that follow provide information about:

- “Model L10 library”
- “Web sites”
- “Getting software updates”
- “Getting help”
- “How to send your comments”

Model L10 library

The following documents contain information related to this product:

- *IBM TotalStorage Storage Switch 2006 Model L10 User's Guide*, GC26-7651-00 (this document)
- *IBM TotalStorage Storage Switch 2006 Model L10 CLI Reference Guide*, GC26-7652-00
- *IBM TotalStorage Storage Switch 2006 Model L10 Quick Reference Card*, GC26-7653-00
- *IBM TotalStorage Storage Switch 2006 Model L10 Statement of Limited Warranty*, GC26-7657-00
- *IBM Safety Notices*, SD21-0030-05

Web sites

You can find additional information related to the software for this and other switches at the following Web site:

<http://www.ibm.com/servers/storage/support/san>

To get specific details about models and firmware that the switch supports, see the following Web site:

<http://www.storage.ibm.com/ibmsan/>

For detailed information about the Fibre Channel standards, see the Fibre Channel Industry Association (FCIA) Web site at:

www.fibrechannel.org/

For a directory of worldwide contact information, including technical support, see the following Web site:

www.ibm.com/contact/

Getting software updates

Contact IBM for software updates and maintenance releases.

Select the SAN support link at the following Web site:

<http://www.storage.ibm.com/ibmsan/index.html>

Getting help

Before contacting technical support, check for solutions in this guide or check with the network administrator.

Online

Contact technical support at the following Web site:

<http://www.ibm.com/servers/storage/support/san/index.html>

Telephone

Within the United States, call 1-800-IBM-SERV (1-800-426-7378).

Outside the United States, go to the following Web site to find the appropriate service number:

<http://www.ibm.com/planetwide/>

How to send your comments

Your feedback is important in helping us provide the most accurate and high-quality information. If you have comments or suggestions for improving this document, you can send us comments electronically by using the following addresses:

- Internet: starpubs@us.ibm.com
- IBMLink™ from U.S.A.: STARPUBS at SJEVM5
- IBMLink from Canada: STARPUBS at TORIBM
- IBM Mail Exchange: USIB3VVD at IBMMAIL

You can also mail your comments by using the Reader Comment Form in the back of this manual or direct your mail to:

International Business Machines Corporation
Information Development
Department GZW
9000 South Rita Road
Tucson, Arizona 85744-0001 U.S.A.

When you send information to IBM, you grant IBM a nonexclusive right to use or distribute the information in any way it believes appropriate without incurring any obligation to you.

Chapter 1. Introduction

The IBM TotalStorage Storage Switch 2006 Model L10 is designed for entry-level storage area networks (SANs), which provide the following advantages over direct attached storage:

- Greater application availability
- Higher performance between servers and storage devices
- Improved storage asset utilization
- Lower storage management and support costs
- Incremental scalability to keep up with difficult to estimate storage growth

This switch is ideal for storage pooling and consolidation, high-performance shared tape library backup and recovery, server clustering, and streaming rich media applications.

Enclosed in a 1U, half-rack form factor enclosure, the switch is built around the InSpeed™ SOC 320 and is controlled by firmware loaded into the on-board flash.

The switch is designed as a central interconnect following the ANSI FC-AL standard. Devices are connected to the switch through small form-factor pluggable (SFP) transceivers and cables. Each attached node has 1 or 2 Gigabits per second (Gb/s) of Fibre Channel bandwidth. The switch operates at full switching bandwidth that reaches speeds of 4 Gb/s per port and up to 40 Gb/s of aggregate bandwidth.

Complete switch configuration and management is available through the intuitive, graphical-based Web Manager interface. A variety of network configurations are easily established using the switch's Port Smart Settings, One-Step Zoning, Automatic Trunking, and Load Balancing features. In addition, the switch features granular change notification management, retained system configuration parameters, and a Command Line Interface (CLI) for advanced users.

Features

The Model L10 storage switch includes the following features:

- High Performance Fibre Channel Switching:
 - Wire speed non-blocking Crossbar switch core
 - Single 10-port InSpeed SOC 320 ASIC with embedded SERDES
 - Multiple simultaneous conversations between ports
 - Traffic routed directly to destination ports
 - 2 Gb/s or 1 Gb/s performance across all ports
 - Aggregate bandwidth of 40 Gb/s
 - Supports one cascade (two switches maximum) and up to 126 host and storage devices
 - No complex fabric services or buffers
- Patent-pending technology:
 - Fairness and Prioritization—ensures that all devices have guaranteed access, or explicitly have prioritized access, over all other devices in a system.
 - Stealth™ Intelligent Change Manager—delivers maximum stability through automatic elimination of state and change notification system disruptions and unprecedented control of disruptive events.
 - Automatic Trunking—enables fully-multiplied throughput and bandwidth, failover pathing, and dynamic load balancing and device prioritization.
- Advanced diagnostics, performance monitoring, and fault isolation including continuous switch and port monitoring and automatic bypass of problematic or unused ports.
- Port Smart Settings, which are predefined port-level configurations that optimize switch performance and stability.
- One-Step Zoning, including overlapping/non-overlapping zones with port or AL_PA-based zoning.
- Switch management using the embedded http-based web server, Command Line Interface (CLI), or Simple Network Management Protocol (SNMP).
- Half-rack, 1U size for easy installation (optional 19" rack-mounting kits available).
- Fibre Channel ANSI Standards Compliance

InSpeed™ technology

InSpeed technology is an advanced switching architecture that couples a non-blocking crossbar switch with a unique switch port logic and per-port SERDES. This results in the industry's highest density Fibre Channel switch on a chip (SOC). The port logic is based on Fibre Channel-Arbitrated Loop (FC-AL), an ANSI standard (X3T11) designed to provide shared bandwidth over low-cost media.

This architecture enables the switch's router to send data directly from one port to another, allowing for multiple, simultaneous conversations between ports—effectively multiplying bandwidth. InSpeed provides the same performance as complex fabric switches that support FC-SW2. InSpeed can even exceed fabric switch performance in entry-level SAN environments, where the overhead associated with longer name addressing and services is not beneficial.

Chapter 2. Switch installation

Installation preparation

After receiving the switch, perform the following steps to ensure that the switch and other contents arrived safely.

To unpack the switch:

1. Inspect the outer shipping container for any damage that may have occurred in shipping. Report any sign of damage to the appropriate shipping agency.
2. Remove the switch and cables from the shipping container; save the shipping container, foam, and antistatic bags—returning the switch in any other container is not advised.

Make sure the following parts are included:

- L10 storage switch unit
 - RS-232 null-modem serial cable
 - Power cable
 - Self-adhesive pads (4)
 - SFP modules (4-pack)
 - Quick Reference card
 - Product Release Notes
 - Safety Notices guide
 - Additional documentation, including warranty information document and the software license agreement.
3. Inspect the switch thoroughly. (If any signs of damage are seen, notify a sales representative and/or the shipping agency.)

Switch installation

The switch can be installed in a rack or placed on a desktop.

Rack installation

Installing the switch in an equipment rack requires an optional rack mount kit (sold separately). The rack mount kit holds two switches. Install the tray with the switch(es) attached into a rack following the instructions provided with the rack mount kit.

Contact a sales representative for more information or assistance in purchasing a kit.

Guidelines for Mounting Equipment in a Rack

When installing equipment in a rack, give careful consideration to the following factors:

- The operating ambient temperature of rack-mounted equipment must not exceed the maximum rated ambient temperature, which is indicated in this installation guide. See “Operating conditions” on page 61.
- The air flow clearances specified in this installation guide must be maintained within the rack. See “Operating conditions” on page 61.
- The AC supply circuit for rack-mounted equipment must be capable of supplying the total current specified on all the labels of the rack-mounted equipment.
- All AC power supply connections must be properly grounded (earthed). To ensure the integrity of the grounded connection, special attention must be given to connections that are not directly connected to the branch circuit (for example, power strips).
- The rack-mounting hardware has been carefully selected to properly support the equipment. Any alternate rack-mounting hardware must provide equal or superior support.
- Plan the device installation starting from the bottom of the rack cabinet. Install the heaviest device in the bottom of the rack cabinet.

Desktop installation

To place the switch on a desktop:

1. Turn the switch upside down so the case bottom is facing up.
2. Install a self-adhesive pad (included) on each corner of the switch bottom approximately 1 inch from each side (prevents surface damage).
3. Turn the switch right-side up so the case bottom is facing down and place the switch on a stable table or platform.

Note: Refer to the “Safety and environmental notices” section and the separate *Safety Information* document for important safety notices regarding the installation and use of this product.

For information on environmental requirements, see “Operating conditions” on page 61.

Switch LEDs

The switch incorporates three sets of light-emitting diodes (LEDs) to indicate Ethernet, switch, and port status:

1. Ethernet LEDs – two separate LEDs indicating the network connection status.
2. System LEDs – four separate LEDs indicating the switch's status.
3. Port LEDs – two LEDs per port indicating the port's status.

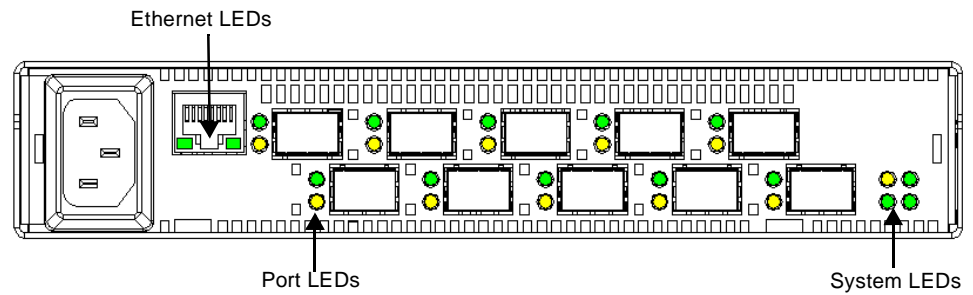


Figure 1. Switch view depicting Ethernet, port, and system LEDs

1100001

Ethernet LEDs

The Ethernet LEDs indicate the network connection status:




Figure 2. Ethernet LEDs

1100002

Table 1. Ethernet LED descriptions

Ethernet LEDs	Indication
Ethernet Activity (green LED)	<ul style="list-style-type: none"> • When flashing, the Ethernet port is receiving data. • When flashing rapidly, the traffic level is high.
Ethernet Link (green LED)	When lit, the switch is connected to an operational Ethernet.

System LEDs

The System LEDs indicate the switch's status, independent of the port LEDs.




Figure 3. System LEDs

Table 2. System LED descriptions

System LEDs	Indication
Fault (yellow LED)	<ul style="list-style-type: none"> When lit, one or more of the ports has failed or the internal temperature has exceeded acceptable levels. When flashing, all ports are operational but another error has occurred. Errors appear in an event log. The level of error severity that will cause flashing to start can be controlled using the <code>config sys fault</code> command in the CLI. The default is level 3, Critical. <p>Note: Whether lit or flashing, the switch will continue to operate. Switch functionality may be impaired depending on the event that triggered the Fault LED. Regardless of the cause, the switch requires immediate attention.</p>
Power (green LED)	When lit, the switch is plugged in and the internal power supply is functional.
2 Gb/s (green LED)	When lit, the switch is set to operate at a speed of 2 Gb/s. When off, the switch is set to 1 Gb/s.
Switch Operational (green LED)	<ul style="list-style-type: none"> When lit, indicates that the switch has completed initialization for ports with inserted SFPs and that the switch is operational. When flashing, the switch has been configured for multiple zones, and one or more zones are up with at least one zone down. <p>If no zones (excluding hard zones) are operational, the LED turns off.</p>

Port LEDs

The Port LEDs indicate the port's status. Each port has two LEDs:

- SFP Status LED
- Port Bypassed LED




Figure 4. Port LEDs

Table 3. Port LED descriptions

SFP Status LED (green LED)	Port Bypassed LED (yellow LED)	Indication
Off	Off	Normal port operational status when an SFP is not installed.
Off	On or Flashing	The port is bypassed due to a faulty or improperly seated SFP. After fixing this problem, power may need to be cycled before the LED indication will change.
Flashing	Off	Activity. Data is being transferred between the port and device.
On	Off	Normal operation but no activity. Port and device are fully operational.
On	Flashing	Manually bypassed. A port can be manually bypassed using the Web Manager's Bypass Port feature.
On	On	Bypassed. SFP is installed but the port is not receiving a valid signal or is receiving an F8 Failure notification from the attached device.
Flashing	Flashing	Beaconing. This is set manually using the Web Manager or CLI.

Serial port

The switch provides a DB-9 serial port on the cosmetic end. The serial port is used to communicate with the switch through the Command Line Interface (CLI).

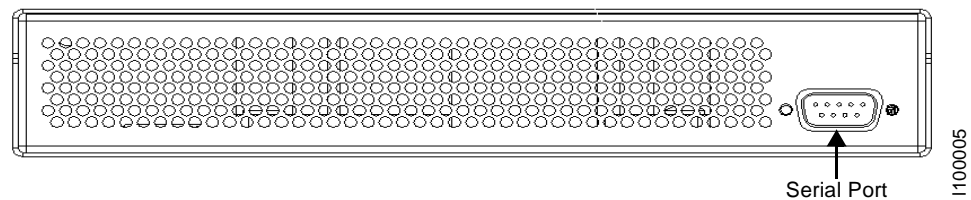


Figure 5. Switch view depicting DB-9 serial port

SFP compatibility

SFPs are “hot-pluggable” into the switch, which allows host computers, servers, and storage devices to be added dynamically without requiring power removal from the switch or any connected devices.

The switch supports small form-factor pluggable (SFP) modules that comply with the SFP specification as produced by the MSA consortium and have passed qualification testing.

The switch ships with a 4-pack of SFP modules. Refer to the *IBM TotalStorage SFP Module Option Installation Guide (GC26-7566)* for additional information.

Installing an SFP

If the Change Notification on Insertion policy is enabled, plugging an SFP into the switch will automatically send an F7 Initialization notification to indicate the device is ready to begin initialization.

Attention: Forcing an SFP into a port may damage the SFP and/or port.

To insert an SFP:

1. Remove dust covers or plugs from the SFPs, if provided.
2. Slide the SFP into the port, ensuring correct polarity, until the latch clicks into place.

Removing an SFP

To extract an SFP:

Determine what kind of extraction mechanism the SFP has and remove the SFP as follows:

- *If the SFP has a removal tag*, remove the cable from the SFP and then pull the removal tag outward and toward the side of the SFP with the tag.
- *If the SFP has a small plastic slider on the top or bottom*, remove the cable from the SFP and then push in the slider and hold while pulling out the SFP.
- *If the SFP has a bale (small metal clasp)*, remove the cable from the SFP and then unlatch, pivot, and pull the bale.

Attaching a device to the switch

To attach a device:

1. Make sure that the device is FC-AL compatible.
2. Attach a cable to the device.
3. Attach the other end of the cable to an SFP.
4. Make sure that the device and switch are operational and set to the same speed.

Booting the switch and SAN

The following procedure is recommended when booting the switch and SAN. Before powering on the switch and SAN, read the Release Notes, included with the switch contents, to determine any modifications that may be required for a specific installation.

To boot the switch and SAN:

1. Power on the storage devices (such as tape libraries and RAID systems).
2. Insert the plug end of the switch's power cord to a properly grounded power source.
3. Insert the power cord's IEC connector end into the switch's power receptacle.

The switch powers on and runs Power-On Self-Test (POST) diagnostics to verify the fundamental integrity of the switch ports. All switch LEDs turn on (LEDs illuminate). Then, excluding the Ethernet Link and Power LEDs, the LEDs turn off (LEDs extinguish). Once the switch is operational, the LEDs display current status as described in "Switch LEDs" on page 7.

Note: The power cord's IEC connector plug serves as the switch's disconnect device. To cycle power to the switch, remove and reconnect the switch's power cord.

4. Power on any other switches connected to the SAN.
5. For certain applications, switch configuration must be completed before continuing with the next step. For information regarding switch configuration, see Chapter 3. Switch management.
6. After all switches have initialized, power on the hosts.

The network initializes.

Note: FC-AL compatible nodes must perform initialization procedures upon power-up in order to function properly. It is the responsibility of the Fibre Channel driver software on FC-AL nodes to perform this initialization.

7. Check all port LEDs.

The SAN should be fully operational at this point. However, it is appropriate to ensure that proper discovery has taken place and all required devices are participating in the network. Some host bus adapters may provide this level of functionality or it might be resident in the application software on the host operating system.

Chapter 3. Switch management

This chapter is divided into three sections providing information on how to manage and monitor the switch:

- Getting started – Describes how to configure the network interface, use the Web Manager, and perform a basic initial setup of the switch.
- Managing the switch – Describes how to configure the switch and port settings, manage firmware versions and configuration files, set switch thresholds, and configure One-Step Zoning, Automatic Trunking, and Load Balancing.
- Monitoring the switch – Describes how to view switch information, the event log, port information, and port diagnostics.

The switch incorporates two distinct interfaces for managing and monitoring purposes:

- The Web Manager interface provides an intuitive graphical user interface that enables you to quickly check switch status or modify switch settings in a visual environment.
- The Command Line Interface (CLI) provides flexibility and additional functionality for advanced users.

Both of these interfaces provide nearly identical functionality; however, for the purposes of this guide, the Web Manager interface is used for switch and port configuration unless otherwise noted.

For a list of CLI commands, see Appendix B. CLI quick reference on page 63. For additional information on the CLI, see the *CLI Reference Guide*.

Getting started

This section explains how to configure the switch's Ethernet network settings prior to using the Web Manager. Once the switch's network settings are configured, use the Web Manager to perform a quick switch setup.

Configuring the network interface

Before using the Web Manager, ensure that the switch's Ethernet network parameter settings are correct for the network configuration. The switch ships with the following default IP settings:

- IP Address: 192.168.1.129
- Netmask: 255.255.255.0
- Gateway: 192.168.1.1

To adjust these settings to open the Web Manager, connect to the switch using the provided serial interface cable and follow the instructions below.

To connect through a serial interface:

1. Attach one end of the included RS-232 null modem cable to the computer's DB-9 serial port and attach the other end to the switch's DB-9 serial port.

2. Open a terminal session through a serial terminal emulation program (such as HyperTerminal®) with the appropriate serial port (for example, COM1) and the following serial port parameters:
 - Bits per second: 19200
 - Data bits: 8
 - Parity: None
 - Stop bits: 1
 - Flow control: None
3. If using HyperTerminal, press ENTER to receive a prompt.
If using the `tip` command on a UNIX workstation, do the following:
 - a. View the `/etc/remote` file and create an alias similar to Hardware but with the serial port parameters above. (Suggested name: Switch)
 - b. Use the `tip` command to establish a connection through the created alias, for example `tip switch`. (For more information, see the `tip` command Manual page.)
4. Type the password at the prompt and press ENTER. (The default password is 'password'.)
5. From the serial terminal emulation program, type `config network ip` and press ENTER.
The switch's current IP parameters are displayed with a prompt for entering the IP address.
6. Change the IP address and press ENTER.
7. Use the `mask` and `gateway` commands to change the subnet mask and default gateway respectively.
8. Type `save` and press ENTER.
9. Type `root reset` and press ENTER.
10. Type `y` and press ENTER to reset the switch.
11. Attach the computer to the switch's 10/100 Ethernet connector by doing one of the following:
 - Attach an Ethernet RJ-45 cross-over cable directly between the computer and the switch.
 - Attach two Ethernet RJ-45 twisted pair cables from the computer and the switch into an operational Ethernet patch panel or hub.

Connecting to the Web Manager

The Web Manager displays current port utilization and health, enables easy to use Port Smart Settings and One-Step Zoning, and several additional features discussed later in this chapter.

Note: The Web Manager supports Microsoft Internet Explorer® for Windows® version 5.5 or later.

To connect to the Web Manager:

1. Ensure that the workstation has access to the network on which the switch is connected.
2. Open Microsoft Internet Explorer.
3. In the address bar, type the switch's DNS name or IP address and press ENTER.

Web Manager overview

The Web Manager enables you to view and configure switch and port settings using an intuitive, graphical user interface. The main page is the Switch Information page. This page displays general switch status and continually refreshes to display the most current switch status. For more information on the Switch Information page, see “Switch information” on page 49

To return to this page at any time, click the **Storage Switch** menu item.

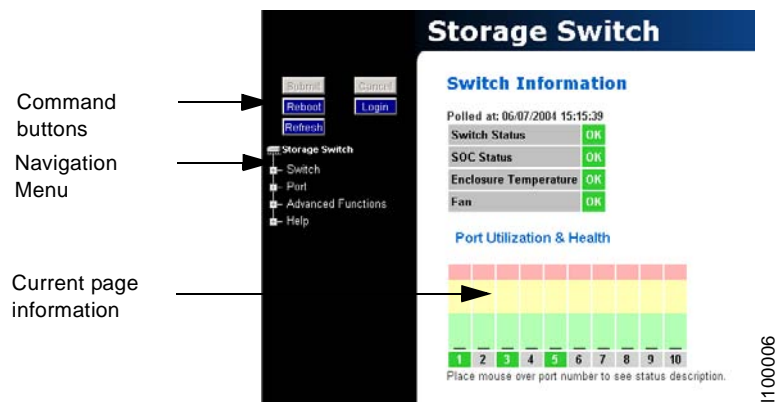


Figure 6. Web Manager interface

Note: The Web browser's appearance and information depends on the switch's active firmware version and may change without notice in subsequent firmware versions.

The Web Manager interface consists of a series of command buttons, an expandable navigation menu, and the displayed information area. The command buttons and navigation menu are always present on the page.

Table 4. Web Manager command buttons

Command Button	Description
Submit	Saves any changes made to the switch configuration. This button is disabled until a configuration setting is changed or new information is entered. This button appears green to indicate a change to the switch configuration. Click this button to accept the configuration change.
Cancel	Cancels a request. This button is disabled until a configuration setting is changed or new information is entered. This button appears green to indicate a change to the switch configuration. Click this button to cancel the configuration change.
Reboot	Resets the switch.
Login/Logout	Logs in to and out of the switch.
Refresh	Redraws the currently displayed web page. You may also press CTRL+F5 to refresh the current Web page.

The expandable navigation menu provides several options for configuring and monitoring the switch. The menu uses a tree-based navigation structure with a list of menu options and items. Clicking a menu option with a "+" next to it expands the menu option and displays additional menu items. Clicking a menu item displays the selected Web Manager page.

To ensure that the most current information is displayed, use the navigation menu instead of the browser's Back and Next buttons, which usually display cached copies and may not reflect current switch information.

To log out of the Web Manager, click **Logout**, or simply close the browser window.

Note: The Web Manager will automatically log you out after 15 minutes of inactivity, unless the Switch Information page is currently displayed. The Switch Information page automatically updates to display the most current switch status.

Documentation

The Web Manager's Help menu provides links to online product documentation and firmware downloads.

To access product documentation and technical briefs, click **Help**, and select **Documentation > Product Docs** or **Technical Briefs**.

To access firmware, click **Help > Downloads**.

Initial switch setup

Once a network connection has been established with the switch and an instance of the Web Manager is open, some basic switch configuration tasks are recommended:

- Log in to the switch.
- Change the switch's password.
- Verify the switch's date and time settings.
- Change the switch's name.

For additional information on Web Manager features and functionality, see "Managing the switch" on page 19 and "Monitoring the switch" on page 49.

Step 1: Log in to the switch

The switch incorporates a password-level security system to prevent unwanted changes to the current switch configuration. In order to make any changes to the switch, you must be logged in to the switch.

To log in to the switch:

1. Click **Login** on any Web Manager page.

A message box appears confirming the login request.

2. Click **OK**.

The switch login page appears.

3. Enter the switch's password.

The default password is 'password'.

4. Click **Log In**.

A message page appears while the page is loading. If the page fails to load in the indicated time, click **Continue**.

See "Logging in to the switch" on page 20 for additional information.

Step 2: Change the password

The default password is set at the factory to 'password'. Change the default password to secure the switch and guarantee that any configuration changes are only performed by registered users.

To change the password:

1. Click **Switch > Password**.

The Switch Password page appears.

2. Enter the new password in the **New Password** text box.

Note: The password must be between 6 and 25 characters in length and is case sensitive.

3. Enter the new password again in the **Confirm New Password** text box.

4. Click **Submit**.

A message box appears confirming the change to the switch's configuration.

5. Click **OK**.

The Password set success message appears confirming that the new password was saved and activated.

See “Changing the password” on page 25 for additional information.

Step 3: Verify the date and time

During the initial Web Manager session, the date and time for the switch are set based on the host system’s current settings.

To view the current date and time:

1. Click **Switch > Date & Time**.

The Switch Date & Time page appears.

To set the date and time settings:

1. Enter the new date and time settings in the appropriate fields.
2. Click **Submit**.

The new date and time appear under Current Date & Time.

To synchronize the current date and time settings with the host system:

1. Click **Host Time**.

The date and time of the current host system appear in the New Date & Time text box.

2. Click **Submit**.

The new date and time appear under Current Date & Time.

See “Configuring date and time settings” on page 24 for additional information.

Step 4: Change the switch name

While not required, changing the switch’s name is recommended for identification and troubleshooting purposes.

To change the switch name:

1. Click **Switch > Configuration**.

The Switch Configuration page appears.

2. Enter the new name in the Name text box.
3. Click **Submit**.

The new name appears in the Name text box and also appears in the title bar.

Note: The Web page may have to be refreshed before seeing the name change. Press **CTRL+F5** to refresh the Web browser instance or open a new Web browser instance.

See “Switch identification” on page 21 for additional information.

Managing the switch

The Model L10 provides several options for managing and configuring the switch to meet the needs of the network environment.

This section describes how to log in to the switch, configure switch and port settings, manage firmware and configuration files, and configure One-Step Zoning, Automatic Trunking, and Load Balancing.

Frequent switch configuration tasks

A list of frequent switch configuration-related tasks is provided below. The list displays the task, the corresponding Web Manager command, and a reference to where more information may be found in this guide.

Table 5. Frequent switch configuration tasks

To...	Click...	In this guide, see...
View switch status	Storage Switch	"Viewing switch status" on page 49.
Change general switch configuration	Switch > Configuration	"Configuring the switch settings" on page 20.
Change the IP Address	Switch > Configuration	"Network location" on page 22
Change the switch speed	Switch > Configuration	"Switch Speed" on page 22.
View the event log	Switch > Event Log	"Viewing the Event Log" on page 51.
Configure traps	Switch > SNMP Traps	"Setting SNMP traps" on page 23.
Upgrade the firmware	Switch > Files	"Switch Firmware Files" on page 35.
Change the Port Smart Settings	Port > Smart Settings	"Configuring the port Smart Settings" on page 27.
Configure One-Step Zoning	Advanced Functions > One-Step Zoning	"One-step zoning" on page 37.
Configure Automatic Trunking	Advanced Functions > Automatic Trunking	"Automatic trunking" on page 45.
Configure Load Balancing	Advanced Functions > Load Balancing	"Load balancing" on page 46.
Reset the switch	Reboot	"Configuring the switch settings" on page 20.

For information on viewing switch status and information, see "Monitoring the switch" on page 49.

Logging in to the switch

The Web Manager requires you to log in to the switch when changes are made to the switch's configuration. Login is not required for viewing switch information.

To log in to the switch:

1. Click **Login** on any Web Manager page.

A message box appears confirming the login request.

2. Click **OK**.

The Switch Login page appears.



Figure 7. Switch Login page

3. Enter the switch's password.

Note: If you do not remember the password, contact a customer service representative.

4. Click **Log In**.

A message page appears while the page is loading. If the page fails to load in the indicated time, click **Continue**.

Configuring the switch settings

Several switch configuration settings may be changed to customize the switch to the network environment. To make a change to the current switch configuration, you must be logged in to the switch or know the switch password (the switch prompts for the password before accepting changes to any configuration settings).

To change a switch setting:

1. Enter new information or make changes to current settings.
2. Click **Submit**.

The Web Manager page displays the new settings or information.

Changes to certain switch settings require that the switch be reset for those changes to occur. You must be logged in to the Web Manager to reset the switch.

To reset the switch:

1. Ensure that any changes to the current switch configuration have been saved.
2. Click **Reboot** on the Web Manager page.

The switch will reset.

General switch settings

The Switch Configuration page displays general settings and switch identification information.

To view the Switch Configuration page, click **Switch > Configuration**.

Setting	Description
Name	Storage Switch
Location	None
Contact Name	IBM Technical Support
Serial Number	IBMSeria001
Ethernet IP Address	192.168.1.129
Netmask	255.255.255.0
Default Gateway	192.168.1.1
MAC ID	00 10 9b 03 05 47
Switch FW Version	2.08 (build 2)
Switch HW Version	2
InSpeed SOC Version	2
MIB Version	1.2
Speed	1 Gb/s 2 Gb/s
Blocking ARB	FF
Agent Up Time	0 days 00:14:24

Figure 8. Switch Configuration page

Switch identification

This section includes general switch identification information.

Table 6. Switch identification settings

Setting	Description
Name	The name of the switch.
Location	The location of the switch.
Contact Name	The person or group to contact about the switch.
Serial Number	A unique identification number assigned to each switch at the factory. This setting can only be configured or modified on Customer Replaceable Units (CRUs).

The name, location, and contact name information may be modified for the network environment. The serial number setting is factory set and cannot be modified.

To change the name, location, or contact name:

1. Click **Switch > Configuration**.
2. Enter the new value in the appropriate text box.
3. Click **Submit**.

The Switch Configuration page displays the updated information.

Network location

The switch's network location is identified by the IP Address, Netmask, and Gateway fields.

Table 7. Network location settings

Setting	Description
Ethernet IP Address	The current IP Address for the switch.
Netmask	The current IP Netmask address for the switch.
Default Gateway	The current Gateway address for the switch.

To change the switch's network location settings:

1. Click **Switch > Configuration**.
2. Enter the new value in the appropriate text box.
3. Click **Submit**.

The Switch Configuration page displays the updated information.

Version information

The different software and hardware versions installed on the switch.

Table 8. Software and hardware version information

Setting	Description
MAC ID	A unique device address (MAC address) assigned to each switch at the factory. This setting cannot be configured or modified.
Switch FW Version	The current firmware loaded onto the switch.
Switch HW Version	The hardware version of the switch. This setting cannot be configured or modified.
SOC Version	The SOC 320 version used in the switch. This setting cannot be configured or modified.
MIB Version	The proprietary Management Information Base version that is supported through SNMP. This setting cannot be configured or modified.

Switch Speed

The Switch Speed setting indicates the current speed per port at which the switch is running. All ports operate at the same speed. The default switch speed is set to 2.125 Gb/s.

To change the switch speed:

1. Click **Switch > Configuration**.
2. Select the desired speed.

Table 9. Switch speed settings

Setting	Description
1 Gb/s	Set switch speed to 1.0625 Gb/s.
2 Gb/s	Set switch speed to 2.125 Gb/s.

3. Click **Submit**.

Blocking ARB

When two ports start a communication session, the Blocking ARB is sent to all other ports trying to communicate with those ports until the connection is terminated. The default setting is "FF". If other connected devices use the "FF" setting for another purpose, select another Blocking ARB value (for example, "FB"). Under normal circumstances, this setting does not need to be modified.

Agent Up Time

The Agent Up Time field displays the duration of time that the switch has been operational. If the switch is rebooted or power is cycled, this value is reset.

The Agent Up Time field is for display purposes and cannot be configured.

Setting SNMP traps

Simple Network Management Protocol (SNMP) uses traps to transmit information to SNMP-based network administration programs. The Switch SNMP Trap Configuration page displays information on the switch's current SNMP trap configuration.

To view the SNMP trap configuration page, click **Switch > SNMP Traps**.

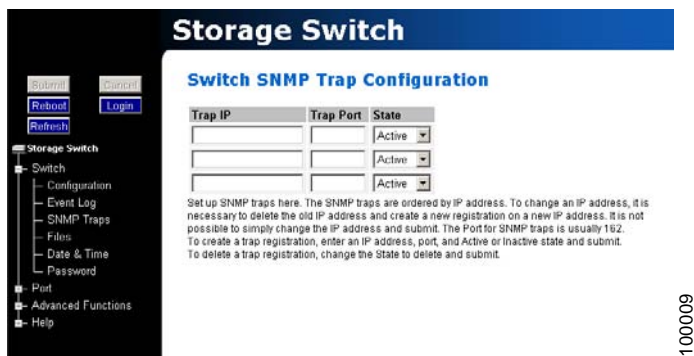


Figure 9. Switch SNMP Trap Configuration page

To configure an SNMP trap:

1. Enter the Trap IP address for the device to which the trap information will be sent.
2. Enter the Trap Port number.

This value is usually set to "162" for Windows.

3. Select the State.

Table 10. SNMP trap settings

State	Description
Active	The trap sends messages to the host identified in the IP Address selection.
Inactive	The trap is not operational.
Delete	The trap will be deleted from the table once changes are saved.

4. Click **Submit**.

When editing a registered IP address, delete the current IP address and create a new entry for the revised IP address.

Configuring date and time settings

The Switch Date & Time page displays the switch's current date and time. During the initial Web Manager session, the date and time for the switch are set based on the host system's current settings. If the switch is rebooted or power is cycled, the system clock will reset and the switch's date and time settings will be set to the host system's time settings of the next user to log in to the switch.

To change the time:

1. Click **Switch > Date & Time**.

The Switch Date & Time page appears.

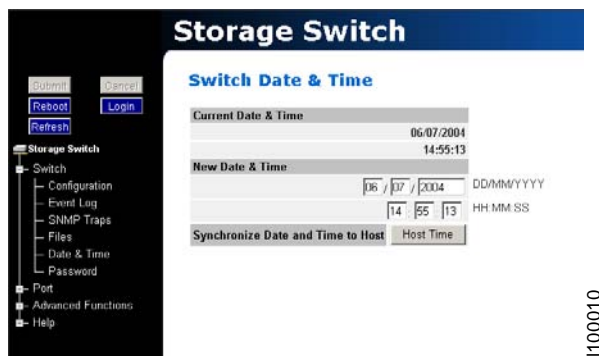


Figure 10. Switch Date & Time page

2. Enter the desired date and time in the appropriate fields.

3. Click **Submit**.

The new date and time appear under **Current Date & Time**.

To synchronize time with the host system:

1. Click **Host Time**.

The date and time of the current host system appear in the **New Date & Time** text box.

2. Click **Submit**.

The new time appears under **Current Date & Time**.

Changing the password

The Switch Password page enables you to change the password for modifying the switch's configuration. The same password is used to access both the Web Manager and the CLI.

Note: Until the default switch password is changed, any user with knowledge of the default password can make changes to the switch's configuration.

To change the password:

1. Click **Switch > Password**.

The Switch Password page appears.



Figure 11. Switch Password page

2. Type the new password in the **New Password** text box.

Note: The password must be between 6 and 25 characters in length and is case sensitive.

3. Type the password again in the **Confirm New Password** text box.
4. Click **Submit**. If you are not logged in to the switch, a password prompt appears requesting that the current password be entered. Enter the current password to proceed.

A message displays confirming that the password was saved and activated.

Opening a telnet session

Some switch operations may require advanced features currently not found in the Web Manager. These features are available in the Command Line Interface (CLI), which can be accessed through the Web Manager by opening a telnet session to the switch.

To open a telnet session with the switch:

1. Click **Advanced Functions > Telnet Session**.

A message box appears confirming the opening of a telnet session to the switch.

2. Click **OK** to proceed.
3. Enter the switch's password and press ENTER.

For additional information on CLI features and functionality, see the *CLI Reference Guide*.

Adjusting the switch thresholds

The Switch Thresholds page displays a variety of switch threshold settings.

Table 11. Switch threshold settings

Setting	Description
Ordered Set Error Threshold	The maximum number of OS errors allowed in a 10-second interval before a port is bypassed. Setting this value to "0" returns it to the factory default setting. This setting is activated on the Port Smart Settings page.
Cyclic redundancy check (CRC) Error Threshold	The maximum number of CRC errors allowed in a 10-second interval before a port is bypassed. Setting this value to "0" returns it to the factory default setting. This setting is activated on the Port Smart Settings page.
Bad Zone Recovery Hold Time (measured in centi-seconds)	The amount of time that the switch keeps the ports in bypass mode before attempting to re-insert the ports into the zone. This setting is activated on the Advanced Functions One-Step Zoning page.
Bad Zone Recovery Delay Time (measured in seconds)	The amount of time that the switch waits after a zone goes down before attempting to recover the zone. This setting is activated on the Advanced Functions One-Step Zoning page.
Port Utilization Interval (measured in seconds)	The length of time between readings of the current port's utilization.

To view the current threshold settings:

Click **Advanced Functions > Thresholds > Switch**.

The Switch Thresholds page appears.

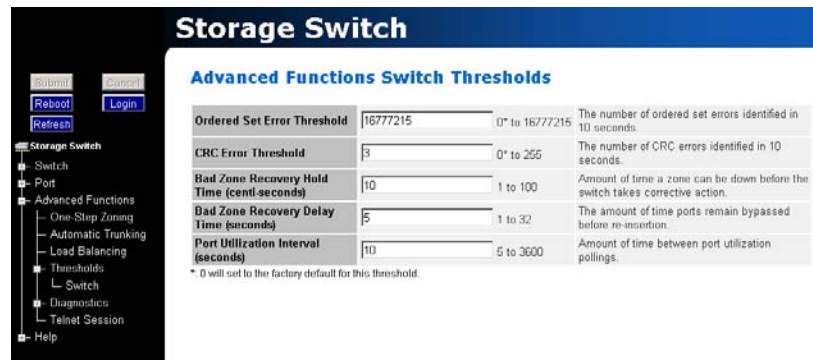


Figure 12. Switch Thresholds page

1100012

To change switch thresholds or time intervals:

1. Enter the new value in the appropriate text box.
The valid range is displayed next to the text box.
2. Click **Submit**.
The new value is set.

Configuring the port Smart Settings

The Port Smart Settings page displays the current Smart Settings (configuration settings) assigned to each port and enables you to easily create and modify custom Smart Settings.

To view the **Port Smart Settings** page:

Click **Port > Smart Settings**.

The Port Smart Settings page appears.

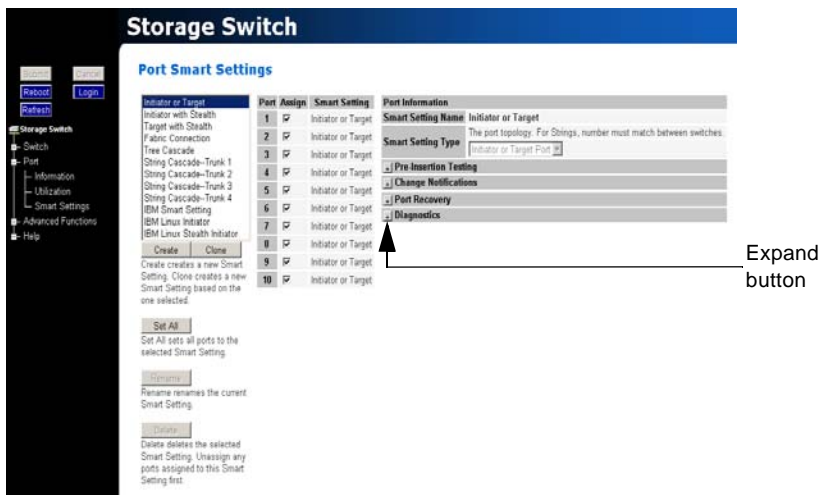


Figure 13. Port Smart Settings page

Expanding the optional configuration menus on the right-side of the page by clicking the expand buttons provides additional configuration options.

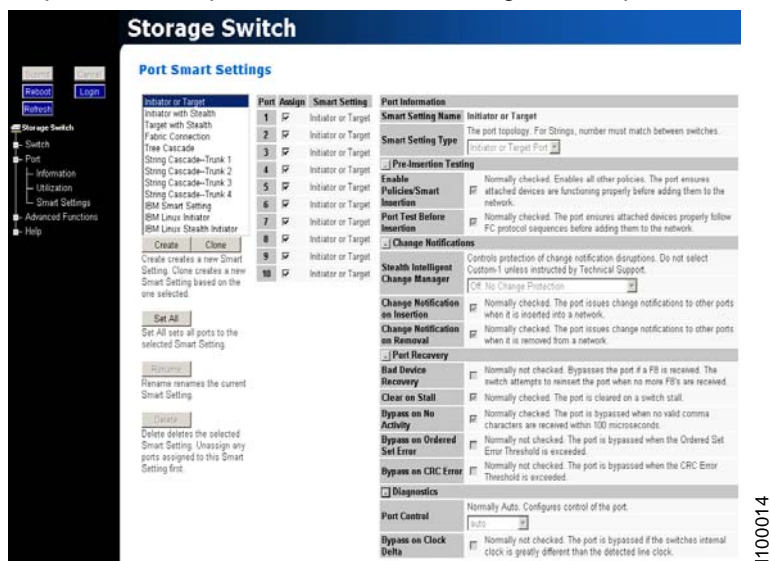


Figure 14. Port Smart Settings page (all options displayed)

Default Smart Settings

There are several default Smart Settings available on the switch. These default Smart Settings were defined by Fibre Channel storage experts to ensure that the switch is optimally configured for performance and stability.

The default Smart Settings cannot be modified or deleted, but these settings can be used as templates for creating custom Smart Settings.

Note: Changing the Smart Setting of a port may affect the performance or behavior of the system. Depending on the implementation, some Smart Settings are more appropriate than others.

Initiator or Target

This Smart Setting is the default setting for all switch ports from the factory. This setting offers no change protection and all settings are set to their default values. Initiators and targets can be connected to ports that are set to this Smart Setting.

This is the recommended Smart Setting for setups with targets and initiators connected to a single switch.

Initiator with Stealth

This Smart Setting is used when connecting a host device to the port. When a port is set to this Smart Setting, change notifications are not sent from the initiator to other devices, but change notifications are received by the initiator.

This Smart Setting is appropriate for embedded storage controllers and external Host Bus Adaptors (HBAs) or servers with installed HBAs.

Target with Stealth

This Smart Setting is used when connecting embedded storage devices, like JBOD enclosures, SBOD™ enclosures, tape drives, or external RAID systems (JBOD enclosures, SBOD enclosures, or tape libraries). When a port is set to this Smart Setting, change notifications are sent to other devices, but change notifications are not received by the target.

Fabric Connection

This Smart Setting is used when connecting a port to a Fabric switch. Only one connection from the L10 storage switch to a Fabric switch is valid.

Tree Cascade

This Smart Setting is used when connecting two or more switches together in a tree configuration. Up to four tree cascades are supported between switches. See “Cascading switches” on page 43 for additional information.

String Cascade

This Smart Setting is used when connecting two switches together in a string configuration. Up to four string cascades are supported between two switches. See “Cascading switches” on page 43 for additional information.

Before selecting a cascade option, consider the following:

- Cascade ports of like number should be connected together. For example, connect port 1 of Switch A to port 1 of Switch B.
- Cascade port numbers must be lower than non-cascade port numbers (for example, Initiator or Target ports). Therefore, select cascade types before selecting these non-cascade types.

- A maximum of two switches may be connected using string cascades.

IBM Smart Setting

This Smart Setting is a custom setting defined by IBM.

IBM Linux Initiator

This Smart Setting is a custom setting defined by IBM that has the Port Test Before Insert (PTBI) policy disabled.

IBM Linux Stealth Initiator

This Smart Setting is a custom setting defined by IBM that has the Port Test Before Insert (PTBI) policy disabled, and the Stealth Intelligent Change Manager feature is enabled and set to “Only Receive Changes”.

To assign a Smart Setting to one or more ports:

1. Select the appropriate Smart Setting from the list box.
2. From the list of port numbers, select the ports that will use the selected Smart Setting under the Assign heading.
3. Once completed, click **Submit** to save the settings.

To set all ports to the currently selected Smart Setting:

1. Select the desired Smart Setting from the list box.
2. Click **Set All**.
3. Click **Submit** to save the new settings.

Creating custom Smart Settings

In addition to the default Smart Settings, you can create custom Smart Settings for use in a specific network environment.

To create a custom Smart Setting:

1. Click **Create**.

A text box appears prompting for the name of the new Smart Setting.

Note: The Create function always uses the Initiator or Target Smart Setting as the base setting from which to configure a custom Smart Setting

2. Enter the new Smart Setting name.

A name may consist of up to 28 alphanumeric characters and cannot contain spaces (use underscores for spaces in names).

3. Click **OK**.

The new Smart Setting is added to the list box.

4. Click **Submit** to save the new Smart Setting.

To create a custom Smart Setting based on an existing Smart Setting:

1. Select a Smart Setting from the list box that most closely matches the port settings that the new Smart Setting should have.
2. Click **Clone**.
3. Enter the new Smart Setting name.

A name may consist of up to 28 alphanumeric characters and cannot contain spaces (use underscores for spaces in names).

4. Click **OK**.

The new Smart Setting is added to the list box.

5. Click **Submit** to save the new Smart Setting.

To modify a custom Smart Setting:

1. Ensure that the custom Smart Setting is not currently assigned to a port before making any changes.
2. Select the custom Smart Setting in the list box.
3. Select the new settings.
4. Click **Submit** to save the new settings.

To rename a custom Smart Setting:

1. Select the desired Smart Setting from the list box.
2. Click **Rename**.
3. Enter the new Smart Setting name.

A name may consist of up to 28 alphanumeric characters and cannot contain spaces (use underscores for spaces in names).

4. Click **OK**.

The new Smart Setting name appears in the list box.

5. Click **Submit** to save the change.

To delete a custom **Smart Setting**:

1. Ensure that the custom Smart Setting is not selected or currently in use.
2. Select the custom Smart Setting in the list box.
3. Click **Delete**.
4. Click **Submit** to save the settings.

Smart Setting assignments

The Smart Settings are based on several port settings grouped into the following categories:

- Port Information
- Pre-Insertion Testing
- Change Notifications
- Port Recovery
- Diagnostics

These settings can be adjusted on custom Smart Settings; however, these settings are fixed on the default Smart Settings.

Port Information

The following settings are available.

Table 12. Port information settings

Setting	Description
Smart Setting Name	Displays the name of the Smart Setting. The Smart Setting name automatically appears in the text box when selected in the scroll menu.
Smart Setting Type	The topology among switches for a port. Options include: <ul style="list-style-type: none">• Initiator or Target Port – the default setting. Should be used when there are no links between switches.• Tree Cascade – designates the port as a tree cascade port. Use this setting when connecting multiple switches together in a tree cascade configuration. Under most conditions, this setting will result in acceptable performance.• String Cascade 1 through String Cascade 4 – designates the string cascade to which a port is assigned. String cascades maintain fairness when two or more InSpeed-based storage switches are serially cascaded. Switch performance may be lower when compared to a tree cascade configuration.

Pre-Insertion Testing

The following settings are available.

Table 13. Pre-insertion testing settings

Setting	Description
Enable Policies/ Smart Insertion	<p>This policy is the default operating mode for all ports and determines what the switch looks for prior to allowing a port to insert into a zone. When the policy is enabled, an external device is sent an F7 Initialization notification by the switch until an F7 Initialization notification is received from the device. Once an F7 Initialization notification is received, the port is inserted in the zone.</p> <p>This policy takes precedence over all other policies. When this policy is disabled, no additional policies are operational, and as long as a port transmits a signal of the correct frequency and amplitude, the port will be allowed in the zone.</p>
Port Test Before Insertion	This policy ensures that a device on a port is a valid, standards-compliant participant before allowing the device to be inserted into a zone. The device must meet all of the FC-AL requirements along with going through a complete change notification cycle. During the change notification cycle, the device becomes the Initialization Master (IM) and goes through the change notification phases. Once the change notification cycle is complete, the device can be inserted. This process ensures that a bad device is not allowed into the zone.

Change Notifications

The following settings are available.

Table 14. Change notification settings

Setting	Description
Stealth Intelligent Change Manager	<p>Stealth Intelligent Change Manager provides stability and control over change notification disruptions on a port basis. Options include:</p> <ul style="list-style-type: none">• Off: No Change Protection – no Stealth Intelligent Change Manager control.• Initiator: Only Receive Changes – devices attached to the port can receive change notifications but will not propagate change notifications generated by that port to other ports.• Target: Only Send Changes – propagates change notifications generated by the port to other ports but will not allow devices attached to the port to receive change notifications from other ports.• Switch-Switch: Send and Receive Changes – allows change notifications to propagate between switches.• Custom-1 – Note: This setting should not be used unless directed to do so by a customer service representative.
Change Notification on Insertion	<p>The switch normally operates under the condition that when a device is inserted onto the network, a change notification is generated. However, this condition is not always true when connecting hubs or switches together. In some instances, it is possible to connect two zones together without the zones realizing that multiple AL_PAs exist with the same values.</p> <p>When this policy is enabled, the switch always generates a change notification to ensure that the proper system updates are performed. However, when a device is removed (for example, an initiator or target), the removal does not generate a change notification and there are no system updates performed.</p>
Change Notification on Removal	<p>This policy is similar to the Change Notification on Insertion policy, except for the change notification being sent when a device is removed rather than inserted.</p> <p>When this policy is enabled, the switch always generates a change notification to ensure that the proper system updates are performed.</p>

Port Recovery

The following settings are available.

Table 15. Port recovery settings

Setting	Description
Bad Device Recovery	<p>When a port is already inserted into a zone, the port transforms F8 Failure notifications into F7 Initialization notifications. When this occurs, the port is bypassed and F7 Initialization notifications are allowed in the zone. Once the initialization is complete, the Bad Zone Recovery Policy is operational and prevents a port that continues to transmit F8 Failure notifications from inserting into the zone.</p> <p>Note: If this policy is disabled while the Bad Zone Recovery policy is enabled, a zone that does go down will still allow the Bad Zone Recovery policy to reset the zone and allow ports to be reinserted.</p> <p>When enabled, this policy prevents devices that send F8 Failure notifications from inserting into a zone. The ability to remove devices that generate F8 Failure notifications automatically and instantaneously guarantees continual system operation.</p> <p>When disabled, this policy allows devices that send F8 Failure notifications to insert into a zone and does not consider F8 Failure notifications when determining whether to insert a device or not.</p>
Clear on Stall	<p>In situations where the switch is operating in switching mode, some devices may fall into an operating mode where the device has opened a target but has not released the connection to the target. When this policy is enabled, the switch can detect this condition and automatically recover when this situation arises.</p>
Bypass on No Activity	<p>The switch detects the amount of time a data stream has gone without receiving a comma. The time setting is set to 100 (.001 seconds). When this policy is enabled, the switch bypasses the disruptive port when the threshold is exceeded.</p>
Bypass on Ordered Set Error	<p>Ordered Set (OS) errors are detected and counted for each individual port. When this policy is enabled, a port is bypassed when its OS count exceeds the threshold setting. The threshold setting is based on the number of ordered set errors identified in 10 seconds.</p> <p>Note: This threshold setting can be adjusted on the Web Manager's Advanced Functions Switch Thresholds page.</p>

Table 15. Port recovery settings (continued)

Setting	Description
Bypass on CRC Error	<p>Cyclic Redundancy Check (CRC) errors are detected and counted for each individual port. When this policy is enabled, a port is bypassed when its CRC count exceeds the threshold setting. The threshold setting is based on the number of CRC errors identified in 10 seconds.</p> <p>User intervention is required to return the port into the zone. Recovery methods include replacing the defective component, cycling power to the device on the port, removing and reinserting the bypassed port, or cycling power to the switch.</p> <p>Note: This threshold setting can be adjusted on the Web Manager's Advanced Functions Switch Thresholds page.</p>

Diagnostics

The following settings are available.

Table 16. Diagnostic settings

Setting	Description
Port Control	<p>The method for controlling a port. Options include:</p> <ul style="list-style-type: none"> • auto – the default setting. The switch will automatically insert a port based on policy settings. This prevents the insertion of incompatible ports, which may cause disruption. • bypass – removes a port from the network. Use this mode to keep a device out of an initialization cycle when troubleshooting. • extLoopback – removes a port from the network and routes the port's receive signal back through the port's transmitter. Use this mode to isolate a specific zone for troubleshooting or to test a transceiver's circuitry and attached media from the node end. • insert – allows ports whose transceivers cannot derive a valid clock or "K" character (Ordered Set) to join a zone. Use this mode cautiously – devices without valid characters may put bad data into a zone, causing the zone to go down.
Bypass on Clock Delta	<p>The switch determines the relative frequency of the signal being received by a port to the internal switch clock. The result of this test allows the determination of how far apart in frequency the switch's clock is in relation to the clock of the received signal – the clock delta. If the clock delta exceeds a set threshold, the switch is notified and the port may be bypassed if necessary. Typically, clock drift is slow enough to allow the removal and replacement of a defective part before the defective part begins to affect system performance.</p>

Managing firmware and configuration files

The Switch Files page displays information on the switch's firmware and configuration files.

To view the firmware and configuration files, click **Switch > Files**.

The Switch Files page appears.

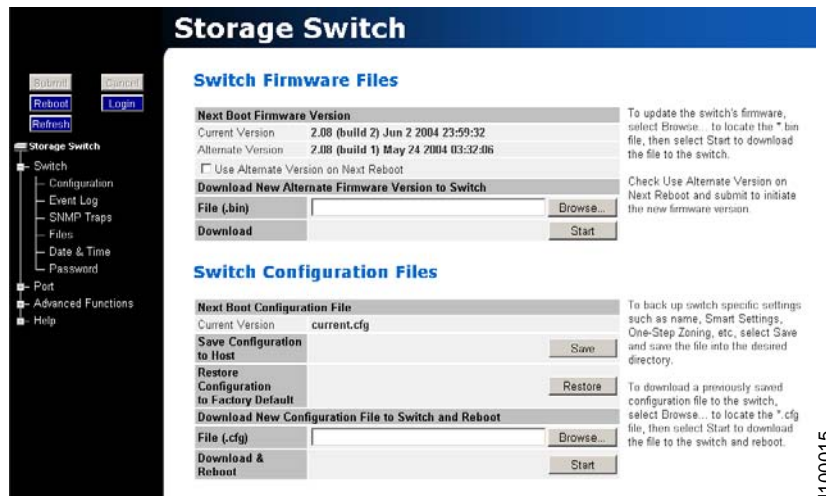


Figure 15. Switch Files page

Switch Firmware Files

This section displays the current and alternate firmware versions, enables you to select which firmware version to run the next time the switch is reset, and provides a means to load new firmware on the switch.

To check for new firmware, click **Help and select Downloads**.

To load new firmware on the switch:

1. Under Download New Alternate Firmware Version to Switch, enter the directory path and the specific file name in the text box, or click **Browse** to navigate to and select the appropriate file on the host system. The file must have a .bin extension.
2. Click **Start** to load the new firmware image.

Once the firmware has been installed, the new firmware should appear as the Alternate Version firmware.

3. Under Next Boot Firmware Version, ensure that the **Use Alternate Version on Next Reboot** option is selected. The alternate firmware version currently displayed will be loaded on the next boot cycle.
4. Click **Reboot** to reset the switch using the selected firmware.

Note: When loading new firmware on the switch, clear the Web browser's cache and files to ensure the removal of the older firmware information. In Internet Explorer, use the key combination **CTRL+F5**, or select **Tools > Internet Options** and click **Delete Files**.

To select the alternate firmware version for the next boot:

1. Under Next Boot Firmware Version, select **Use Alternate Version on Next Reboot**. The alternate firmware version currently displayed will be loaded on the next boot cycle.
2. Click **Submit**.
3. Click **Reboot** to reset the switch.

Switch Configuration Files

Switch configuration settings (for example, zoning or Port Smart Settings) can be saved for backup purposes or for loading the same configuration on multiple switches.

To save the current configuration:

1. Click **Save** to save the current switch configuration.
2. Click **OK** on the File Download dialog box.
3. Enter the directory path and file name, being sure to use a .cfg extension.
4. Click **Save**.

To load a saved configuration:

1. Under Download New Configuration File to Switch and Reboot, enter the directory path to the .cfg file in the text box, or use the **Browse** button to navigate to the appropriate file.
2. In the Choose File dialog box, navigate to and select the appropriate file and click **OK**.
3. Click **Start**.
A message box appears confirming the download and required switch reset.
4. Click **OK** to proceed.

Restoring the factory default settings

If necessary, the switch settings can be reset to their factory default values; however, the network configuration and port type settings are retained.

To restore the factory default configuration:

1. From the Restore Configuration to Factory Default section, click **Restore**.
A message box appears confirming the request.
2. Click **OK** to restore the factory default configuration and reset the switch.

One-step zoning

Zoning allows ports to be divided into multiple virtual zones (or work groups), similar to Virtual Local Area Networking (VLAN). By separating activity on the network, zoning also eliminates change notification propagation (change notifications that occur within one zone cannot propagate to other zones.)

Use zoning to:

- Separate different operating system environments.
- Temporarily block or grant access during backup or other tasks.
- Consolidate equipment logically.
- Designate closed user groups for increased security.
- Separate test or maintenance areas from production areas.

Zone configuration settings are available on the Web Manager's One-Step Zoning page. The page is arranged as a grid of check boxes for placing ports in appropriate zones. Ports are listed across the top of the grid. Zones are listed down the left side. Similar to other Web Manager pages, the port color represents the current port status.

To view the One-Step Zoning page:

Click **Advanced Functions > One-Step Zoning**.

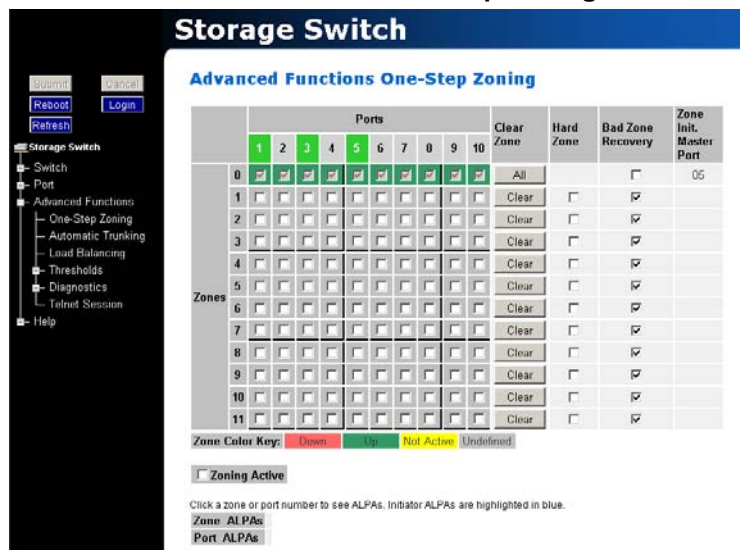


Figure 16. One-Step Zoning page

The switch is capable of up to twelve zones. Initially, all ports reside in Zone 0. However, a port will clear from Zone 0 whenever it is selected and placed in another zone.

The color of each zone indicates its status. See the descriptions in the following table.

Table 17. Zone color status

Color	Description
Down (red)	One or more ports have been selected, zoning has been activated, but hardware has caused a failure.

Table 17. Zone color status

Color	Description
Up (green)	Ports have been selected, zoning has been activated, and the FC-AL circuit is operational.
Not Active (yellow)	Ports have been selected but zoning has not been activated.
Undefined (gray)	No ports have been selected.

The Zone Initialization Master Port field displays the port number of the port that is currently assigned as the master for that particular zone. The Initialization Master is responsible for starting the change notification process in each zone.

To add ports to a zone:

1. Select the appropriate check boxes to place ports into zones.
2. Click **Submit**.

To activate zoning:

1. Select the **Zoning Active** check box near the bottom of the page.

Attention: Clearing the Zoning Active check box will deactivate all zones, which may degrade system performance or compromise security.

2. Click **Submit**.

To remove a port from a zone:

1. Clear the appropriate check box.
2. Click **Submit**.

To remove all ports from a zone:

1. Click **Clear** at the end of the row of check boxes for the appropriate zone.
2. Click **Submit**.

To remove all zones:

1. Click **All** under the Clear Zone heading.
2. Click **Submit**.

Single-switch zoning

The simplest zoning configuration is to place each port into a single zone, so that zones are separate from each other as shown in Figure 17.

The screenshot shows the 'Storage Switch' interface with 'Advanced Functions One-Step Zoning' selected. The main area is a table with 11 zones and 10 ports. Zone 1 is highlighted in blue, indicating it is active. The table shows that Zone 1 includes ports 1, 3, and 4, while Zone 2 includes ports 2 and 5. All other zones are empty.

Zones	Ports										Clear Zone	Hard Zone	Bad Zone Recovery	Zone Init. Master Port
	1	2	3	4	5	6	7	8	9	10				
0	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	All	<input type="checkbox"/>	<input type="checkbox"/>	
1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	01
2	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	02
3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
4	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
5	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
6	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
8	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
9	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
11	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Zone Color Key: Down (red), Up (green), Not Active (yellow), Undefined (grey)

Zoning Active

Click a zone or port number to see ALPAs. Initiator ALPAs are highlighted in blue.

Zone ALPAs
Port ALPAs

1100017

Figure 17. Devices in a single zone

In Figure 17, zone 1 includes ports 1, 3, and 4, while zone 2 includes ports 2 and 5. Devices on ports 1, 3, and 4 have direct access to each other and devices on ports 2 and 5 have direct access to each other; however, devices 1, 3, and 4 are separated from devices 2 and 5.

The screenshot shows the 'Storage Switch' interface with 'Advanced Functions One-Step Zoning' selected. The main area is a table with 11 zones and 10 ports. Zone 1 is highlighted in blue, indicating it is active. The table shows that Zone 1 includes ports 1, 3, and 4, while Zone 2 includes ports 2 and 5. All other zones are empty.

Zones	Ports										Clear Zone	Hard Zone	Bad Zone Recovery	Zone Init. Master Port
	1	2	3	4	5	6	7	8	9	10				
0	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	All	<input type="checkbox"/>	<input type="checkbox"/>	
1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	01
2	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	02
3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
4	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
5	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
6	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
8	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
9	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
11	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Zone Color Key: Down (red), Up (green), Not Active (yellow), Undefined (grey)

Zoning Active

Click a zone or port number to see ALPAs. Initiator ALPAs are highlighted in blue.

Zone ALPAs
Port ALPAs

1100018

Figure 18. Single switch zoning configuration

Adding devices to multiple zones

In the single-switch zoning example, each host only communicates with the devices in the same zone as the host. However, there may be situations in which hosts in separate zones need to share devices. When this situation occurs, use overlapping zones to share the devices between the hosts. Figure 19 depicts this type of zoning configuration.

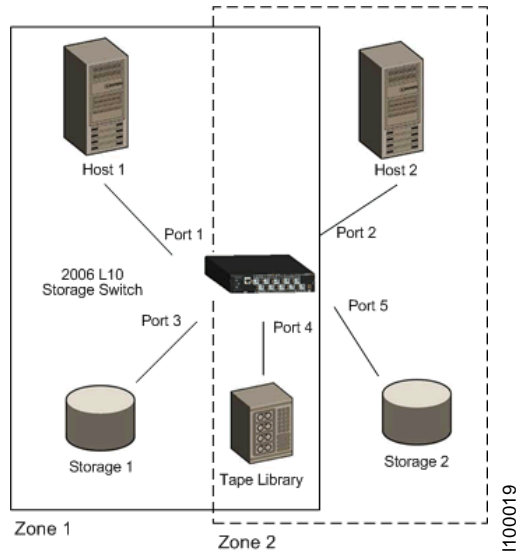


Figure 19. Devices in multiple zones

In Figure 19, zone 1 includes ports 1, 3, and 4, while zone 2 includes ports 2, 4 and 5. Port 4 is in both zones. Devices on ports 1, 3, and 4 have direct access to each other and devices on ports 2, 4, and 5 have direct access to each other, but devices 1 and 3 are separated from devices 2 and 5. The device on port 4 has direct access to all the devices on ports 1, 2, 3, and 5.

To add storage devices to multiple zones:

1. Select the appropriate zones for each port.
2. Ensure that the Zoning Active check box is selected.
3. Click **Submit**.

Storage Switch

Advanced Functions One-Step Zoning

	1	2	3	4	5	6	7	8	9	10	Clear Zone	Hard Zone	Bad Zone Recovery	Zone Init. Master Port
0	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	All	<input type="checkbox"/>	<input type="checkbox"/>	
1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	03
2	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	05
3	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
4	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
5	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
6	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
8	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
9	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
11	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Clear	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Zone Color Key: Down (Red), Up (Green), Not Active (Yellow), Undefined (Grey)

Zoning Active

Click a zone or port number to see ALPAs. Initiator ALPAs are highlighted in blue.

Zone ALPAs
Port ALPAs

Figure 20. Ports in multiple zones on the One-Step Zoning page

Multiple switch zoning

Zones can be configured across multiple switches using a similar procedure to a single switch. However, multiple-switch zoning requires some coordination between the switches.

Note: To ensure zone integrity when configuring multiple switch zoning, you **must** implement AL_PA zoning through the Command Line Interface (CLI). See “AL_PA zoning” on page 42 for additional information.

Building on the example for ports in multiple zones, move the devices onto two switches and have the zones stretch between the two, as in Figure 21.


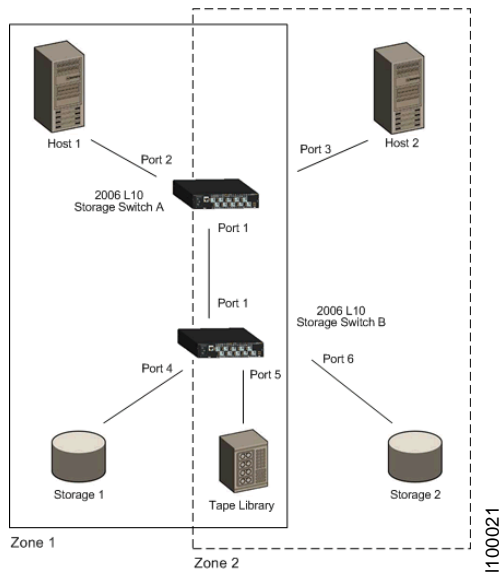


Figure 21. Devices in multiple zones across multiple switches

In Figure 21, zone 1 includes ports 2, 4, 5, and cascade port 1, while zone 2 includes ports 3, 5, 6, and cascade port 1. Ports 1 (cascade port) and 5 are in both zones.

To configure multiple-switch zoning, do the following for each switch:

1. Plan which ports should belong in each zone.
2. From the One-Step Zoning page, select the appropriate ports for each zone.

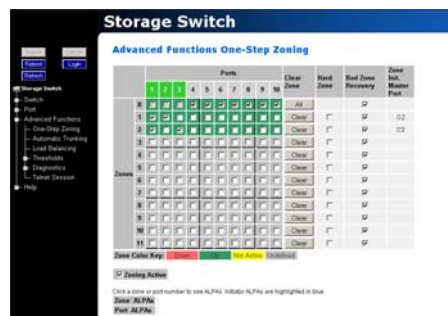

Switch A



Switch B

Figure 22. Zones coordinated on multiple switches

3. Ensure that the Zoning Active check box is selected for both switches.

Attention: Clearing the **Zoning Active** check box will deactivate all zones, which may degrade system performance or compromise security.

4. After making changes, click **Submit**.

AL_PA zoning

AL_PA zoning is a specific zoning configuration that prevents devices from accessing one another. AL_PA zoning fully ensures that devices will not access each other by blocking a group of devices (using AL_PAs) from communicating with each other; however, AL_PA zoning allows the devices to communicate with devices outside of the group.

AL_PA zoning is only accessible through the Command Line Interface (CLI). Refer to the *CLI Reference Guide* for additional information.

Recovering a bad zone automatically

Bad zone recovery policy automatically recovers traffic if a device has brought down the zone. The zone state is monitored continuously. If ports are inserted into a zone, but the zone state never transitions to the Zone Up or Zone Active state after a set period of time (Hold Time), all devices in the pertinent zone are bypassed and then allowed to reinsert. There is a secondary timeout, the Bad Zone Recovery Delay Time, that can also be configured. The Bad Zone Recovery Delay Time causes a delay before ports are allowed to reinsert, which prevents a high “thrashing” level of port insertions and de-insertions and ensures that some devices can reset. The Bad Zone Recovery Hold Time and Delay Time threshold settings are available on the Advanced Functions Switch Thresholds page.

When this policy is enabled with the associated PTBI policy, the device causing a zone to go down is not allowed back into the zone due to the PTBI policy, which allows the system to return to normal operation. The combination of the Bad Zone Recovery and PTBI policies has resulted in significant improvements to SAN availability.

Note: The Bad Zone Recovery policy is enabled by default. If the Bad Zone Recovery policy is disabled, use the following instructions to enable this policy for the appropriate zones.

To activate bad zone recovery:

1. Click **Advanced Functions > One-Step Zoning**.
2. Under Bad Zone Recovery, select the check boxes for the appropriate zones.
3. Click **Submit**.

Connecting ports through Hard Zoning

A Hard Zone can be used to add a separate 126 AL_PAs that operate in isolation from any other zone. A Hard Zone disables switching functionality and creates a shared connection between the ports in a zone topology, splitting the switch into multiple unique FC-AL zones. When Hard Zoning is enabled, all switch zones must be Hard Zones. A combination of Hard Zones and regular zones on a single switch is not allowed.

Attention: Do not set a Hard Zone for ports in multiple zones or share ports that have the Hard Zone option set. This will cause errors that do not log an event or display a message.

The advantages of Hard Zoning include:

- Each Hard Zone contains 126 available AL_PAs.
- The switch can be configured to contain up to eleven isolated Hard Zones.

The limitations of Hard Zoning include:

- 2 Gb of shared bandwidth over the entire Hard Zone.
- Ports in a Hard Zone cannot use the Stealth Intelligent Change Manager.
- Automatic Trunking and route blocking are not allowed in a Hard Zone.
- Ports in a Hard Zone cannot be set to a string or tree cascade configuration.
- Device AL_PAs on a port in a Hard Zone cannot be displayed.

The Hard Zone setting is available on the One-Step Zoning page. To view the page, click **Advanced Functions > One-Step Zoning**.

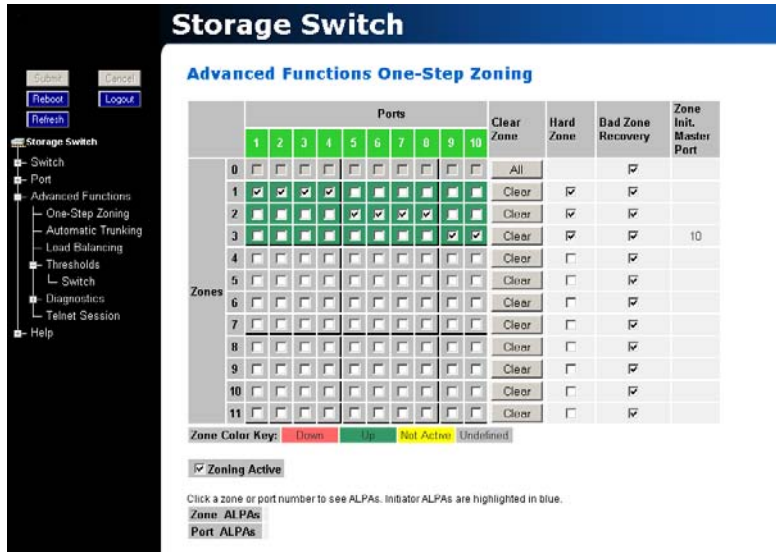


Figure 23. Hard Zoning configuration

1100024

To set up Hard Zoning:

1. Determine which ports will reside in each Hard Zone and ensure that the ports are in only one Hard Zone.
2. Under Hard Zone, select the check boxes for the appropriate zones.
3. Click **Submit**.

Cascading switches

When multiple switches are connected, the connecting links between the switches are referred to as “cascades”. There are two distinct cascade configurations to consider when configuring networks for optimal performance and connectivity: string cascades and tree cascades.

String cascades

A string cascade connects multiple switches (up to two switches maximum) together in a “daisy-chained” configuration. When one device requests access to another device, the request is sent to each switch in the cascade before device access is granted. This arbitration method promotes fairness between the switches. However, when compared to tree cascades, string cascades offer less performance due to the increased latency between the switches.




Figure 24. String cascade configuration example

When configuring a switch port for a string cascade, use the String Cascade Smart Setting. To enable the string cascade, go to the Automatic Trunking page. From the Automatic Trunking page, select the Single Cascade option, or place the string cascade into a trunk group. See “Automatic trunking” on page 45 for additional information.

To reduce contention and improve performance between initiator traffic and target traffic when using a string cascade configuration, connect the ports of each switch together using the same String Cascade Smart Settings. For example, in Figure 24 the two switches are connected through two string cascades using the String Cascade - Trunk 1 and String Cascade - Trunk 2 Smart Settings. This creates two dedicated paths through which initiators and targets can communicate.

Tree cascades

Tree cascades provide the best performance (lowest latency) configuration. A tree cascade consists of a root switch connected to additional switches (up to 8 switches maximum). When a device on a switch requests access to another device, the request is sent the particular switch for that device. The limitation to the tree cascade configuration is the random nature of devices gaining access to one another, as fairness is not used for tree cascades.

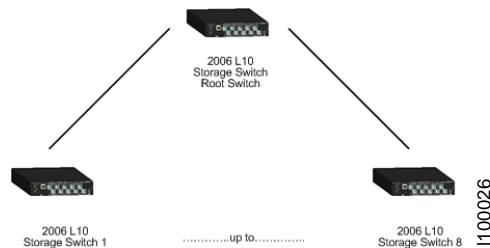


Figure 25. Tree cascade configuration example

When configuring a port for a tree cascade, use the Tree Cascade Smart Setting. To enable the tree cascade, go to the Automatic Trunking page. From the Automatic Trunking page, select the Single Cascade option, or place the tree cascade into a trunk group. See “Automatic trunking” on page 45 for additional information.

Automatic trunking

Multiple links between switches are called “trunks”. Trunks provide higher bandwidth across cascaded switches for systems incorporating multiple initiators. Each trunk can improve system throughput and provide “failover” capability. A maximum of 4 trunks between each switch is supported. Trunking is performed automatically when ports are configured properly. Figure 26 is an example of Automatic Trunking.

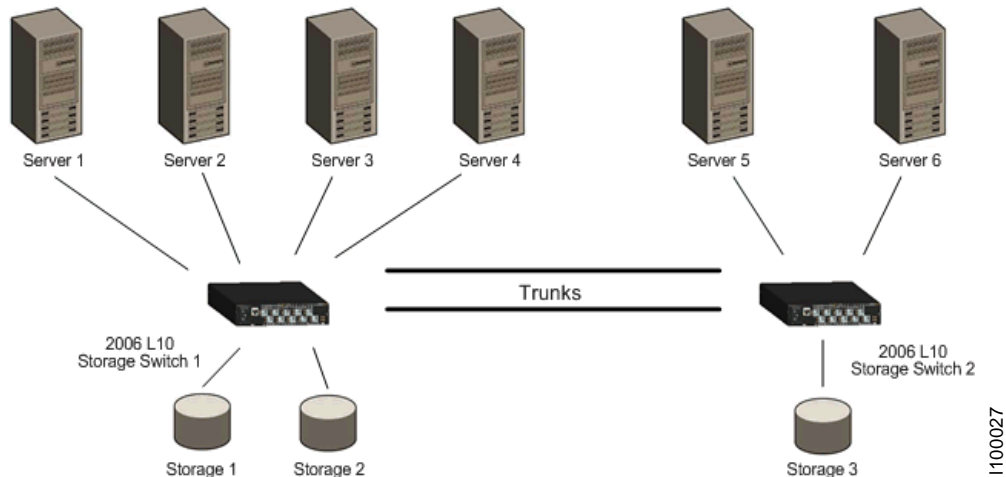


Figure 26. Automatic Trunking example

Each trunk is part of a trunk group. A trunk group consists of two or more cascades between two switches, and these cascades must be the lowest numbered ports on both switches. There can only be one trunk group between two switches. Each trunk group contains a primary trunk. All traffic flows through the primary trunk on a switch unless specified otherwise using the Load Balancing feature. The primary trunk is always the lowest numbered port of any trunk group.

If the primary trunk fails, the secondary trunk automatically becomes the primary trunk unless otherwise configured. Multiple cascades also enable switch configuration for better performance through load balancing (see “Load balancing” on page 46).

The Automatic Trunking page enables you to configure trunking by defining trunk groups and assigning ports to those groups. The Automatic Trunking feature is available when one or more ports are assigned a String or Tree Cascade Smart Setting.

Only one of the three following options may be selected for each port.

- Device or Initiator – Select this option to designate a specific port as an initiator or device. The specified port is not assigned to a trunk group. The Device or Initiator option is the default setting.
- Single Cascade – Select this option when connecting two switches with a single cascade. The selected port is not part of a trunk group.
- Trunk Group – Select this option when multiple cascades are connected between two switches. The selected port must be assigned to an available trunk group. Multiple trunk groups appear when two or more ports are assigned to the same string cascade Port Smart Setting (for example, String Cascade - Trunk 1).

Note: Before changing the Port Smart Setting for a particular port assigned to a trunk group, you must remove that port from the trunk group by selecting the Device or Initiator setting. Remember to click **Submit** to update the port's setting.

To assign ports to a trunk group:

1. Click **Advanced Functions > Automatic Trunking**.

The Automatic Trunking page appears.

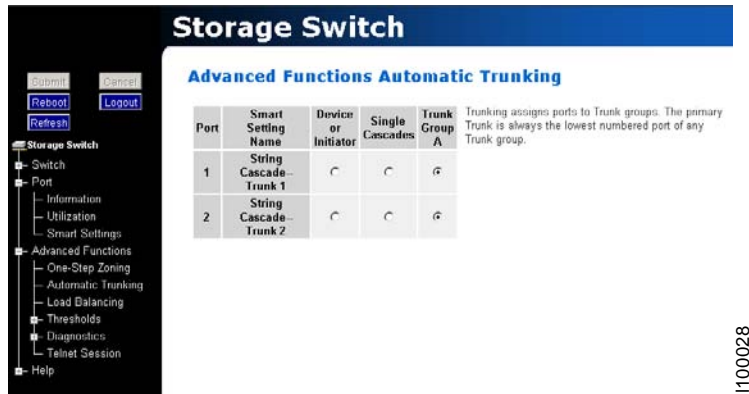


Figure 27. Advanced Functions: Automatic Trunking page

2. Select a trunk group for each port by clicking the appropriate Trunk Group option.
3. When finished making changes, click **Submit**.

Load balancing

Load balancing builds on the Automatic Trunking functionality by specifying the path that an initiator uses to send data between multiple switches. You can manage the switch's aggregate bandwidth by manually distributing traffic across multiple cascade ports. A cascade port is a port that is attached to another switch of the same type and configured as a String or Tree Cascade Smart Setting on the Port Smart Settings page. All data flows through the primary cascade, unless the switch is configured differently.

Note: Cascade ports must be properly configured before load balancing will work.

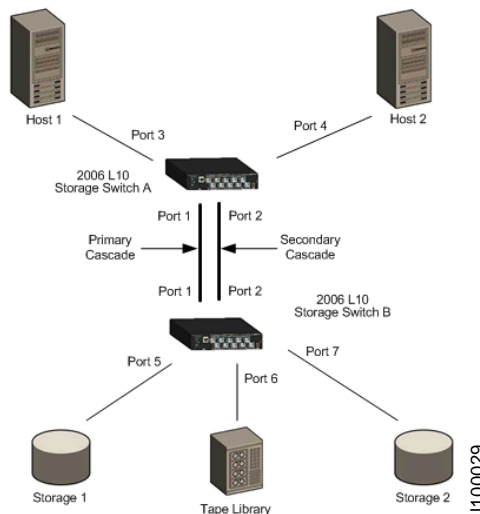


Figure 28. Load balancing across multiple cascade ports

In Figure 28, host 1 uses cascade port 1, while host 2 uses cascade port 2. All traffic will use the lowest numbered (primary) cascade port by default but ports may be configured to use other cascades.

Note: When tape drives or tape libraries are included in multiple switch configurations incorporating multiple trunks, place the tape drive or tape library and any devices that access those devices on the secondary (duplicate) trunk, not the primary trunk.

Load balancing configuration settings are available on the Web Manager’s Load Balancing page. Before implementing load balancing on the switch, the automatic trunking settings must be configured. See “Automatic trunking” on page 45 for additional information.

To view the Load Balancing page:

Click **Advanced Functions > Load Balancing**.

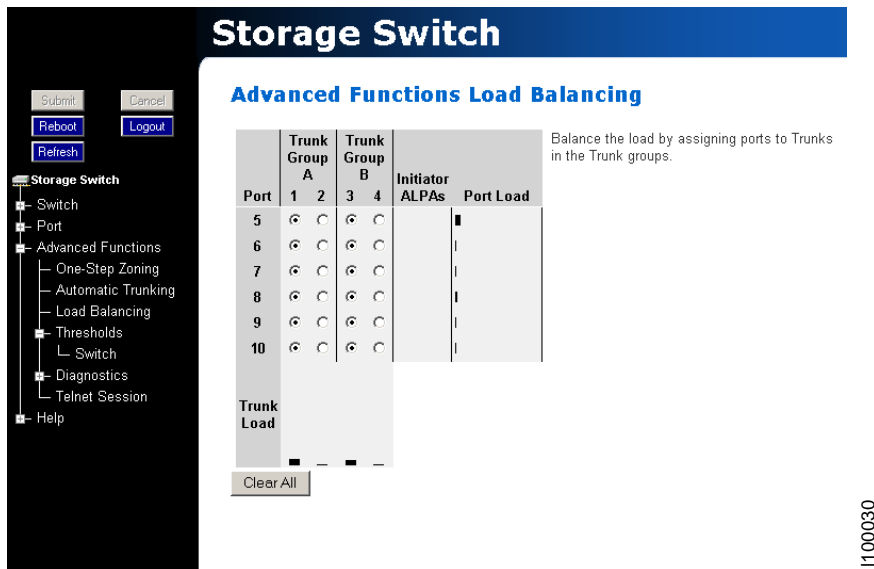


Figure 29. Advanced Functions: Load Balancing page

The page is arranged as a grid of check boxes for assigning ports to cascades (“Trunk Groups”).

Load indicators

The Load Balancing page incorporates two sets of visual indicators for measuring traffic:

- Port Load Indicators—the horizontal bars on the right side of the page that display the current load for each port.
- Trunk Load Indicators—the vertical bars at the bottom of the page that display the current load for each trunk group.

These bars indicate the amount of traffic across a trunk or port. The size of the bars increase in correlation to the amount of traffic and, as a bar’s size increases, can identify a specific trunk or port that is overloaded. If overloading occurs, move one or more ports to a different trunk in the group.

To change the load balancing settings:

1. Click a Trunk Group option to place a port into a specific trunk group.

2. Continue to assign ports to trunk groups as necessary.
3. When finished, click **Submit**.

Fairness and prioritization

The concept of “fairness” is based on the principle of ensuring fair device access and communication across all devices in a storage system. The switch incorporates fairness and prioritization through InSpeed technology and Automatic Trunking and Load Balancing functionality. In cooperation with each other, these features ensure even and equal access through multiple links fairly—effectively multiplying bandwidth.

Device prioritization can be achieved using Load Balancing and assigning only a specific device port to a particular cascade. This ensures that a specific device will always have a dedicated trunk.

Monitoring the switch

The L10 storage switch provides several options for monitoring the switch status and port information. This section describes how to view switch status, the event log, port information and utilization, and port diagnostics.

Viewing switch status

The Web Manager's home page is the Switch Information page. This page is displayed first when the Web Manager is opened and shows general switch information, including switch status, fan and power supply operational indicators, and port health and utilization.

This page continually refreshes to guarantee that the most current switch status is displayed. To return to this page at any time, click the **Storage Switch** menu item.

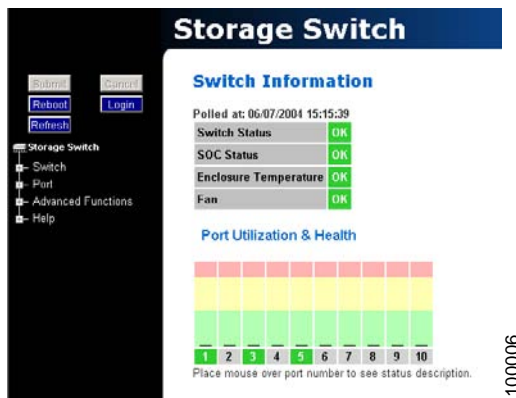


Figure 30. Switch Information page

Switch information

Current status is provided for the following items.

Table 18. Switch status information

Item	Status Indicators
Switch Status	<ul style="list-style-type: none">OK (green)—the switch unit is operating normally.Fault (red)—one or more of the ports has failed, the internal temperature has exceeded acceptable levels, or another error has occurred. Errors appear in the event log. The switch will continue to operate; however, functionality may be impaired depending on the event that triggered the error. Regardless of the cause, the switch requires immediate attention.
SOC Status	<ul style="list-style-type: none">OK (green)—the switch chipset is operating normally.Fault (red)—the switch chipset's selftest has failed.
Enclosure Temperature	<ul style="list-style-type: none">OK (green)—the switch temperature is within the normal operating range.OverTemp (red)—the enclosure temperature has exceeded the recommended operating range.
Fan	<ul style="list-style-type: none">OK (green)—the fan unit is working properly.Fault (red)—the fan unit has stopped operating.

Port utilization and health

Port utilization measures the amount of traffic passing into a port over a period of time. For example, if an initiator is transmitting data to a target, the initiator port displays a port utilization value (%) while the target port does not. If the same initiator is receiving data from the target, the target port displays a port utilization value (%) while the initiator port displays does not.

This part of the web page displays each port number, the port's current health status, and a vertical bar indicating the port utilization.

Note: Rolling the mouse cursor over the port number displays the current port state.

A port number is displayed in one of three colors depending on the port's current health:

Table 19. Port number colors and indications

Port Color	Indication
Green	An SFP is inserted into the port and a device is connected to the SFP.
Yellow	<ul style="list-style-type: none"> • Bypassed – The port is bypassed. An SFP may be inserted in the port but a device is not connected to the SFP. • Loopback – There is no device connected to the port. The transmit and receiver are connected together on the SFP transceiver. • LIPF8Present – If the switch is receiving an F8 Failure notification, the port is bypassed to allow remaining devices to proceed with initialization. • Redundant – The port is a failover link in a cascade and is not currently active.
Red	<ul style="list-style-type: none"> • TxFault – Detects an SFP transmitter fault. • DiagTx – Detects Ordered Sets being transmitted, so traffic cannot be passed through the port. • DataTimeout – Detects a data timeout fault. • RxLoss – Detects a loss of received signal amplitude from the device. • SyncLoss – Detects a loss of word synchronization for a specified time, which may be caused by poor signal strength, intermittent line conditions, etc.
Gray	<ul style="list-style-type: none"> • Unknown – The port status cannot be determined. • NoSFP – There is no SFP connector inserted in the port.

Port utilization is measured by a vertical bar that moves upwards as utilization increases. The vertical bar has the three distinct levels of utilization:

Table 20. Port utilization colors and indications

Bar Color	Indication
Green	The port is operating at optimal utilization.
Yellow	The port is experiencing periods of heavy traffic.
Red	The port has too much traffic on it and is not operating at desired levels. Some devices should be transferred to other ports to improve port utilization.

Viewing the Event Log

The Event Log contains a list of up to 3000 event log messages generated by the switch. The Switch Event Log page displays the event log messages with each message containing the following information:

- Event Number – the number assigned to that specific event in the log.
- Event Date and Time – the date and time when the event was recorded in the log.
- Event Severity – the severity level for that event.
- Event Type – the identifier assigned to that event.
- Event Description – a brief description of the event.

For a complete list of event messages and severity levels, see Appendix C. Event messages on page 67.

To view the event log, click **Switch > Event Log**.

The Event Log Messages page appears.

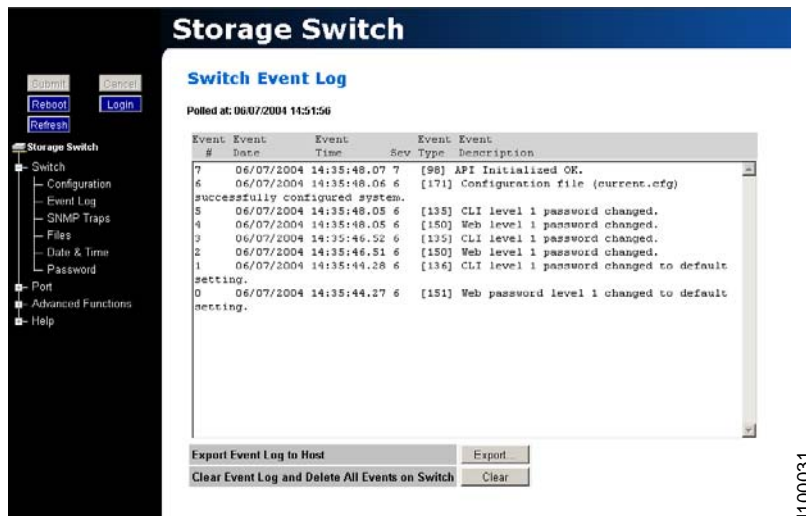


Figure 31. Switch Event Log page

The last time the event log was polled appears at the top of the page.

To export the event log:

1. Click **Export**.

If the File Download dialog box appears, select **Save this file to disk**, and click **OK** to save the file on the host system. The Save As dialog box appears. Select the appropriate directory, change the file name if necessary, and click **Save**.

The event log appears in the host system's default text editor.

2. Select the appropriate directory to save the event log messages, change the name of the file (if desired), and save the event log.

To delete the current list of event log messages on the switch:

1. Click **Clear**.

A message box appears confirming the request.

2. Click **OK** to delete the event log.

The event log is cleared out and a new event message is displayed reporting that the event log has been cleared.

Viewing port information

The Port Information page displays the Smart Settings, Serial ID (SID), and AL_PAs currently assigned to each port. Initiator AL_PAs are highlighted in blue to differentiate them from target AL_PAs.

Note: The Initiator AL_PA information can be used to easily identify attached devices when configuring load balancing.

To view port information, click **Port > Information**.

The Port Information page appears.

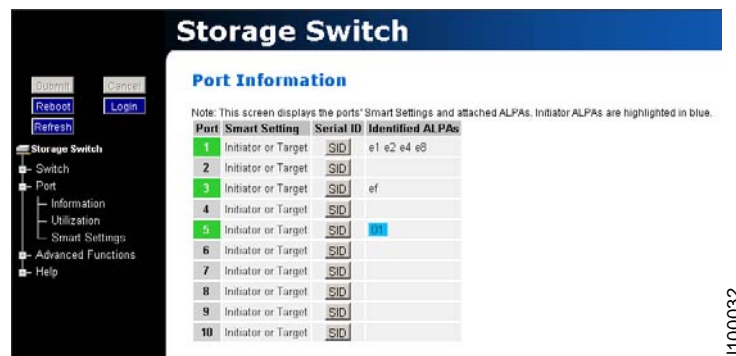


Figure 32. Port Information page

Table 21. Port information settings and descriptions

Field	Description
Port	Displays the current health of the port. See “Port utilization and health” on page 50 for additional information on port health.
Smart Setting	Displays the specific Smart Setting assigned to a particular port. See “Configuring the port Smart Settings” on page 27 for more information on the Smart Settings.
Serial ID (SID)	When clicked, provides additional information about the SFP inserted in the port, if an SFP is inserted in that particular port.
Identified AL_PAs	Displays all the AL_PAs attached to the port. Initiator AL_PAs appear highlighted in blue.

Viewing port utilization

Port utilization measures the amount of traffic passing through a port over a period of time. For example, if an initiator is transmitting data to a target, the initiator port displays a port utilization value (%) while the target port does not. If the same initiator is receiving data from the target, the target port displays a port utilization value (%) while the initiator port displays does not.

The Port Utilization page displays each port’s utilization percentage based on high, average, and low utilization.


Table 22. Port utilization values and descriptions

Value	Description
High	The highest percentage of data communication through a port over a period of time (measured in seconds).
Average	The average percentage of data communication through a port over a period of time (measured in seconds).
Low	The lowest percentage of data communication through a port over a period of time (measured in seconds).

To change the port utilization interval, click **Advanced Functions > Thresholds > Switch**. See “Adjusting the switch thresholds” on page 26 for additional information.

To view port utilization, click **Port > Utilization**.

The Port Utilization page appears.

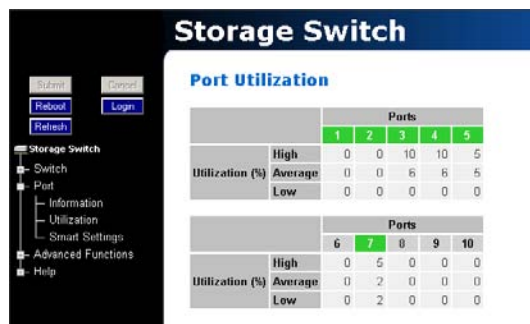

1100033

Figure 33. Port Utilization page

Viewing port diagnostics

This page displays diagnostic information pertaining to each port in the switch. Use the information provided on this page to diagnose abnormally high error counts on a particular port.

To view the current diagnostic settings, click **Advanced Functions > Diagnostics > Port**.

The Port Diagnostics page appears.



1100034

Figure 34. Advanced Functions: Port Diagnostics page

Table 23. Port statistics and descriptions

Statistic	Description
Port & Health	Color Indicators <ul style="list-style-type: none"> • Green • Yellow • Red See "Port utilization and health" on page 50 for descriptions of the health indicators.
Insertion Count	Number of times this port has been inserted into the network since the switch was reset or the counters were cleared.
CRC Errors	Number of CRC errors that are detected in frames passing through this port since the switch was reset or the counters were cleared.
Ordered Set Errors	Number of Ordered Sets that are received on this port with an encoding error since the switch was reset or the counters were cleared.
Clock Delta	Difference (in parts per million) between the internal switch clock and the received clock signal on the port.
State	Current state of this port – either inserted or bypassed.
Beacon Port	Forces both port LEDs to flash on and off continuously. Use this to locate and take action on a specific port. The flashing overrides normal port indication until beaconing is turned off; however, port operation continues to operate normally.
Bypass Port	A single instance operation that forces a port into bypass mode. This feature may be used to diagnose device problems when a device is locked up or experiencing a high number of failures on a port.
Reset Port	A single instance operation that places a port in bypass mode and then immediately sets the port to auto-detect to re-insert the port. This feature may be used to diagnose device problems when a device is locked up or experiencing a high number of failures on a port.

To save diagnostic information:

1. Click **Upload** to save the current diagnostics to the host system.
2. Click **OK** on the File Download dialog box.
3. Enter the directory path and file name.
4. Click **Save**.

To clear the counters, click **Clear**.

Manual port operation

If necessary, a port can be placed into manual bypass mode or reset.

- If the port is placed in bypass mode, the port will remain in bypass mode until the switch is reset.
- If the port is manually reset, the port is temporarily placed in bypassed mode and then reset to re-insert the port.

These features may be used to diagnose device problems when a device is locked up or experiencing a high number of failures on a port.

To place a port into bypass mode:

1. Click **Advanced Functions > Diagnostics > Port**.
2. Select the Bypass Port option for the appropriate port.
3. Click **Submit**.

To reset a port:

1. Click **Advanced Functions > Diagnostics > Port**.
2. Select the Reset Port option for the appropriate port.
3. Click **Submit**.

Viewing ordered sets

This page displays the ordered sets that are being transmitted on the switch for each port since the last time the page was displayed. Ordered sets are used when communicating data across networks to indicate actions, events, or status regarding the data. A list of detected ordered sets and their indications is provided below.

To view ordered sets, click **Advanced Functions > Diagnostics > Ordered Sets**.

The Ordered Sets page appears.

Ordered Set	Ports									
	1	2	3	4	5	6	7	8	9	10
End of Frame	*	*	*	*	*					
Start of Frame	*	*	*	*	*					
Idle	*	*	*	*	*					
ARB(FF)	*	*	*	*	*					
ARB	*	*	*	*	*					
Read Ready	*	*	*	*	*					
Close	*	*	*	*	*					
Open	*	*	*	*	*					
F0 Failure	*	*	*	*	*					
F7 Initialization	*	*	*	*	*					
Change Notification	*	*	*	*	*					
Unknown										
Invalid Word										
CRC Error										
Point to Point										

Figure 35. Advanced Functions: Ordered Sets page

Table 24. Ordered sets and descriptions

Detection	Indication
End of Frame (EOF)	An End-of-Frame (EOF) delimiter has been detected; frames are present. (An EOF immediately follows the CRC of a frame and signals the frame's end.)
Start of Frame (SOF)	A Start-of-Frame (SOF) delimiter has been detected; frames are present.
Idle	Sequences of IDLEs are being transmitted to maintain link activity; no other data is being transmitted.
ARB(FF)	ARB(FF)s are being transmitted to maintain link activity; no other data is being transmitted.
ARB	A port is arbitrating for network access to perform a task.
Read Ready (RRDY)	The receiving node on this port has sent an R_RDY signal, indicating that it is ready for a frame to be transmitted over the link.
Close (CLS)	The port is attempting to begin the process of closing the current FC-AL circuit.
Open (OPN)	The port is attempting to open communications with another port. Note: As is the case with some ordered sets, an OPN may not go all the way around the FC-AL, instead stopping at its destination.
F8 Failure	A non-switching port has detected a failure on its receive input, is notifying other ports, and is determining whether the network is still operational. Some events that could cause the port to detect network failure follow: <ul style="list-style-type: none"> • A device has failed or has been powered off. • The physical connection between the transmitter and receiver is broken. • Activating the port bypass circuit does not typically result in a network failure.
F7 Initialization	A port is in the non-participating mode and is attempting to win arbitration and begin initialization, possibly because the port was reset or is powering up. Sometimes the port is sending this sequence to another hot-cascaded switch, like a new initiator being inserted in the network.
Change Notification	A change notification has been detected and action has been taken.
Unknown	The switch cannot determine what is being transmitted.
Invalid	An invalid transmit word has been detected.
CRC Error	A Frame CRC error has been detected.
Point-to-Point	A point-to-point connection has been detected.

Chapter 4. Technical reference

Troubleshooting device connections

Table 25. Device connection issues and recommended actions

Problem	Recommended Action
SFP installed in one or more ports, but no LEDs lit	<ol style="list-style-type: none">1. Verify that the power cord is firmly seated into switch and is connected to a properly earthed receptacle (outlet).2. Check the Power LED to ensure that the switch is turned on.3. Verify that the SFP is firmly seated.
SFP installed, but only yellow LED is lit	Reseat the SFP. If the same condition occurs, the SFP is probably faulty and should be replaced.
SFP installed with both green and yellow LEDs lit	<ol style="list-style-type: none">1. Make sure that the device is powered on and operating properly.2. Unplug the fiber cable from the node and verify that an optical signal is present on the cable receiver lead.3. Verify that the fiber cable is fully seated at either end. If optical power meter is available, verify the device is transmitting a signal. If there is no signal present, the device may require rebooting, device drivers may need to be reinstalled, or the HBA or disk controller hardware may require servicing. If a signal is present on both the cable lead and the end node, the HBA or disk controller may require service.4. Ensure that the device and switch are operational and set to the same speed.
SFP installed with only green LED lit, but devices are not communicating	<p>The switch is receiving a valid signal from the device, but no upper level protocols are active.</p> <ol style="list-style-type: none">1. Verify that the proper HBA device drivers are loaded for the appropriate operating system and that the host has been configured to recognize attached disk devices.2. Improper FC-AL initialization could result from a defective or inoperative adapter card or device. Run adapter diagnostics with a loopback connector to see if the adapter is working properly.3. Unplug the fiber cable from the end node and verify that an optical signal is present on the cable receiver lead. If no signal is present, the cable's receiver lead may be bad and the device may be streaming F8 Failure notifications.

Troubleshooting management connections

Table 26. Management connection issues and recommended actions

Problem	Recommended Action
Serial cable installed, but connection does not appear on terminal	<ol style="list-style-type: none"> 1. Cycle power by reinstalling the power cord. 2. Check the terminal emulation program's serial port parameters. 3. Replace the serial cable (verify it is a null-modem cable.)
Ethernet cable installed, but Web Manager does not appear	<ol style="list-style-type: none"> 1. Ensure that a crossover Ethernet cable is used (unless using an Ethernet hub). 2. Check the IP addresses on the switch and workstation as follows: At a command line prompt, type ping DNSorIP (where DNSorIP is the switch's DNS name or IP address) and press ENTER. If a "Reply from..." or "...is alive..." message appears, the devices can communicate. If a "Request timed out" message appears (or the command times out), the devices cannot communicate. Trace the cabling. If needed, reconnect the devices.

Port bypass conditions and recovery

Table 27. Port bypass conditions and recovery

Operational Condition	Recovery
Rx_los is asserted by an SFP/GBIC	The port stays bypassed until rx_los is de-asserted. At that time, the port insertion will be automatically retried. The port continues to stay bypassed until the port can pass the port insertion criteria.
Tx_fault is asserted by an SFP/GBIC	The port stays bypassed until tx_fault is de-asserted. At that time, the port insertion will be automatically retried. The port continues to stay bypassed until the port can pass the port insertion criteria.
F8 Failure notification is received by the port (when the LIP F8 Recover policy is enabled)	The switch automatically tries to re-insert the device, by sending F7 Initialization notifications to the device connected to the bypassed port. The port continues to stay bypassed until the device returns F7 Initialization notifications to the port and passes the port insertion criteria.
Loss of Sync (>100ms)	The port stays bypassed until a signal is re-established. At that time, the port insertion will be automatically retried. The port continues to stay bypassed until the port can pass the port insertion criteria.
Firmware Initiated	The port stays bypassed until the firmware sets the port control back to automatic. At that time, the port insertion will be automatically retried. The port continues to stay bypassed until the port can pass the port insertion criteria.

Default Smart Setting attributes

Table 28. Default Smart Setting attributes

	Initiator or Target	Initiator with Stealth	Target with Stealth	Fabric Connection	Tree Cascade	String Cascade --Trunk 1	String Cascade --Trunk 2	String Cascade --Trunk 3	String Cascade --Trunk 4	IBM Smart Setting	IBM Linux Initiator	IBM Linux Stealth Initiator
Cascade Type	nonCascade	nonCascade	nonCascade	tree	tree	string0	string1	string2	string3	nonCascade	nonCascade	nonCascade
Control	auto	auto	auto	auto	auto	auto	auto	auto	auto	auto	auto	auto
Transmitter	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
LIP on Insert Policy	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
LIP on Removal Policy	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
Device Test Before Insert Policy	enabled	enabled	enabled	disabled	disabled	disabled	disabled	disabled	disabled	enabled	disabled	disabled
LIP (F8) Recover Policy	disabled	enabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled
SEOC Policy	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled
Smart Insertion Policy	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
Clear on Stall Policy	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
Bypass on No Comma Policy	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled	enabled
LIP Control	rxtxlip	rxlip	txlip	rxtxlip	nolip	nolip	nolip	nolip	nolip	rxtxlip	rxtxlip	rxlip
Bypass on OS Error Policy	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled
Bypass on CRC Error Policy	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled
Bypass on Clock Delta Policy	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled	disabled

Appendix A. Specifications

Switch specifications

Table 29. Switch specifications

Specification	Value
Number of Ports	10
Operating Rate	All ports operate at 1.0625 or 2.125 Gbps (selectable)
Port Media Type	SFP
Enclosure	1U half-rack form-factor
Management Interface	RS-232 or 10/100 Ethernet
Operating Mode	Switching or Non-switching modes
Configurability	Management interface configurable
Power On Selftest (POST)	Yes
Dimensions	215.9 mm x 39.9 mm x 406.4 mm (W x H x D) (8.50 in. x 1.57 in. x 16.00 in.)
AC Power Input	50 or 60 Hz / 100 – 250 VAC / 0.6 – 0.4 A
AC Power Connector	IEC connector
Weight	Approximately 7 lbs.

Operating conditions

The switch must be operated in a clean, dry environment with unrestricted airflow. Air flows in through the non-port end and out through the port end (sometimes called the transceiver end or “back-of-box”).

To avoid overheating, maintain a minimum clearance of 50.8 millimeters (two inches) on each end of the switch (the non-port end and the port end). Allow an adequate amount of space on the top and sides of the switch for proper air ventilation. Do not place the switch on heat-generating surfaces. Operating conditions are listed below.

Table 30. Operating conditions

Requirement	Value
Operating Temperature	0°C to 40°C normal operation (ambient air temperature)
Storage	-40°C to 80°C non-condensing
Power	50 or 60 Hz / 100 – 250 VAC / 0.6 – 0.4 A

Appendix B. CLI quick reference

Connecting to the CLI

The Command Line Interface (CLI) can be accessed through a network interface using a terminal emulation program, such as HyperTerminal, or through the serial interface from a local computer. Refer to the *CLI Reference Guide* for detailed descriptions of CLI commands and usage.

To connect through a network interface:

Use a network terminal emulation program. For example, if using the telnet command on a Windows workstation, type telnet *IPaddress* at a command prompt.

To connect through a serial interface:

1. Attach one end of the included RS-232 null modem cable to the computer's DB-9 serial port, and attach the other end to the switch's DB-9 serial port.
2. Open a terminal session through a serial terminal emulation program (such as HyperTerminal) with the appropriate serial port (for example, COM1) and the following serial port parameters:
 - Bits per second: 19200
 - Data bits: 8
 - Parity: None
 - Stop bits: 1
 - Flow control: None
3. If using HyperTerminal, press ENTER to receive a prompt.
4. If using the tip command on a UNIX workstation, do the following:
 - a. View the */etc/remote* file and create an alias similar to Hardware but with the serial port parameters above. (Suggested name: Switch)
 - b. Use the tip command to establish a connection through the created alias, for example tip switch.

Logging in and out

The CLI does not require login if only viewing basic system information. However, for viewing detailed system information or configuring any switch settings, you must log in to the switch.

To log in to the CLI:

Type `li`, type the password at the prompt, and press ENTER. (The default password is 'password'.)

To log out of the CLI:

Type `lo` and press ENTER, or exit the terminal session.

Using the CLI

The CLI enables you to monitor and change system and port configurations, configure One-Step Zoning, Automatic Trunking, Load Balancing, and event reporting parameters, and download and install firmware.

For additional information on the CLI, see the *CLI Reference Guide*.

To enter a command, type the command text or the number of the command.

To return to the previous menu, type `..` and press ENTER.

To return directly to the Root menu, type `root` and press ENTER.

To cancel a prompt or input request, press ENTER.

To display help for specific command, type `? <command>` and press ENTER.

To save changes to the switch configuration at any time:

1. Type `save` at any command prompt and press ENTER.
A message appears confirming the request.
2. Type `y` and press ENTER.

Frequent switch configuration tasks

A list of frequent switch configuration-related tasks is provided below. The list displays the task and the corresponding CLI command.

Table 31. Switch configuration tasks

To...	Type...
View switch status	<code>show sysinfo</code>
Change general switch configuration	<code>config sys</code>
Change the IP Address	<code>config network ip</code>
Change the switch speed	<code>config sys speed</code>
View the event log	<code>show events</code>
Upgrade the firmware	<code>fw</code>
Change the port settings	<code>config port</code>
Configure zoning	<code>config zone</code>
Configure trunking	<code>config load</code>
Configure load balancing	<code>config trunk</code>
Reset the switch	<code>reset</code>
Perform diagnostics	<code>diag</code>
Reset the switch to factory default settings	<code>config default</code>
Change the password	<code>config password</code>

CLI commands

All of the CLI commands for the Model L10 are shown below in a tree diagram. Using the “help” command at the command line may provide additional information.

Table 32. CLI command quick reference

root --> help li lo save	1. config -->	1. save				
		2. sys -->	1. speed	8. lipen	15. fault	
			2. mode	9. name	16. evclr	
			3. oserr	10. location	17. clrled	
			4. crcerr	11. contact	18. ..	
			5. blkarb	12. syslog	19. ?	
			6. clkd	13. events		
			7. time	14. sev		
			3. default			
			4. port -->	1. beacon	5. view	9. ..
				2. show	6. edit	10. ?
		3. types	7. del			
		4. add	8. type			
	5. password					
	6. load -->	1. show	5. delalpa	9. pu1		
		2. lbclr	6. addalpa	10. pu2		
		3. delprt	7. ialpa	11. ..		
		4. addprt	8. util	12. ?		
	7. trunk -->	1. addprt	3. showmem	5. ..		
		2. delprt	4. clr	6. ?		
	8. network-->	1. reset	4. mask	7. ?		
		2. show	5. gateway			
		3. ip	6. ..			
	9. zone -->	1. bzht	7. deact	13. hz		
		2. bzdt	8. zstate	14. bzs		
		3. addprt	9. zclr	15. alpas		
		4. delprt	10. addblk	16. ..		
		5. showmem	11. delblk	17. ?		
		6. act	12. showblks			
	10. ..					
	11. ?					
	2. diag -->	1. galpa	5. delta	9. beacon		
		2. glim	6. showpri	10. con		
		3. os	7. prtctrs	11. who		
		4. ps	8. clrctr	12. ialpa		
	3. show -->	1. events	6. sysinfo	11. glim		
		2. ptype	7. zninfo	12. sensors		
		3. portinfo	8. lbinfo	13. getcon		
		4. prtctrs	9. os	14. sync		
		5. clrctr	10. galpa	15. dump		
	4. fw -->	1. tftp	3. revert	5. reset		
		2. xmodem	4. show	6. ..		
	5. reset					
	6. ?					

Appendix C. Event messages

The event messages for the switch are listed below. For explanations, contact a customer service representative. The message's applicable severity level as defined below is also provided.

Table 33. Event message severity levels

Severity Level	Severity	Description
1	EMERG	Immediate action required; system failing
2	ALERT	Unrecoverable condition reported; major event in progress
3	CRIT	Event failed with possible loss of integrity
4	ERR	Condition failed; action required
5	WRN	Failed event occurred; no action required
6	NOTIFY	Configuration error or abnormal event occurred; no action required
7	INFO	Event occurred; no action required

These severity levels can be used to designate which events trigger trap messages. Use the Command Line Interface (CLI) to designate the minimum severity level of events to be logged in the Event Log and at which severity level to illuminate the switch's Fault LED.

Table 34. Event message information

Event	Event Message	Severity
1	Message log cleared	INFO
5	Power Supply Failed	ALERT
6	Power Supply Online	NOTIFY
9	Fan has stopped	EMERG
10	Fan has returned	ALERT
19	Temperatures over limit	ALERT
20	Temperature OK	INFO
50	SPF Overvoltage	EMERG
54	SOC has detected a CRC error in the EEPROM	NOTIFY
70	PORT # bypassed	NOTIFY
71	PORT # inserted	NOTIFY
72	Transceiver detected at port #	NOTIFY
73	Transceiver removed at port #	NOTIFY
74	SEOC occurred on PORT #	NOTIFY
75	Port exceeded OS threshold	NOTIFY
76	Port exceeded CRC threshold	NOTIFY
77	Loop UP on Port #	NOTIFY
78	Loop DOWN on Port #	NOTIFY
79	PORT received a LIP(F8)	WRN

Table 34. Event message information (continued)

Event	Event Message	Severity
80	PORT CRC Error detected in frame	WRN
81	PORT did not receive LIPF7) within timeout	WRN
83	Segment stall on PORT #	NOTIFY
84	Bad Open on PORT #	WRN
85	Error during Port Disc.	NOTIFY
86	PORT PTBI failed due to timeout	NOTIFY
87	PORT changed to STATE	NOTIFY
88	Transceiver in PORT has been cycled	NOTIFY
89	PORT has cycled between insert/bypassed (not necessarily in that order)	NOTIFY
90	Loop CYCLED on Port #	NOTIFY
91	Port exceeded Clk Delta threshold	INFO
95	Interframe has been received	INFO
96	Interswitch link added/removed	INFO
97	LIP Cycle Timeout	INFO
98	API Initialized OK	INFO
99	Selftest failure	ERR
100	Received Unknown event	INFO
101	CRC detected on either an ISL LIP or Generic Frame	NOTIFY
107	Trap task failed to update trap destination info.	CRIT
135	CLI level 1 password changed	NOTIFY
136	CLI level password changed to default setting	NOTIFY
150	WEB level 1 password changed	NOTIFY
151	Web password level changed to default setting	NOTIFY
165	System config reset to factory default	ERR
166	New Port Config Type added	NOTIFY
167	Port Config Type deleted	NOTIFY
168	Current Config saved to flash	NOTIFY
169	Error in saving config file to flash	ERR
170	Error in retrieving config information	ERR
171	Config File successfully configured system	NOTIFY
172	Error in initializing system with config file	ERR
198	A device tried to access another device that was not in the same zone	NOTIFY
199	Health timer has expired on ZONE	NOTIFY
208	PORT is over threshold	NOTIFY
218	Trunk DOWN on PORT #	NOTIFY
219	Trunk UP on PORT #	NOTIFY
220	New Primary Trunk	NOTIFY

Appendix D. AL_PA cross references

Table 35. AL_PA cross references

Arbitrated Loop Physical Addresses								
AL_PA	AL_PA ID		AL_PA	AL_PA ID		AL_PA	AL_PA ID	
(hex)	(hex)	(decimal)	(hex)	(hex)	(decimal)	(hex)	(hex)	(decimal)
EF	00	0	A3	2B	43	4D	56	86
E8	01	1	9F	2C	44	4C	57	87
E4	02	2	9E	2D	45	4B	58	88
E2	03	3	9D	2E	46	4A	59	89
E1	04	4	9B	2F	47	49	5A	90
E0	05	5	98	30	48	47	5B	91
DC	06	6	97	31	49	46	5C	92
DA	07	7	90	32	50	45	5D	93
D9	08	8	8F	33	51	43	5E	94
D6	09	9	88	34	52	3C	5F	95
D5	0A	10	84	35	53	3A	60	96
D4	0B	11	82	36	54	39	61	97
D3	0C	12	81	37	55	36	62	98
D2	0D	13	80	38	56	35	63	99
D1	0E	14	7C	39	57	34	64	100
CE	0F	15	7A	3A	58	33	65	101
CD	10	16	79	3B	59	32	66	102
CC	11	17	76	3C	60	31	67	103
CB	12	18	75	3D	61	2E	68	104
CA	13	19	74	3E	62	2D	69	105
C9	14	20	73	3F	63	2C	6A	106
C7	15	21	72	40	64	2B	6B	107
C6	16	22	71	41	65	2A	6C	108
C5	17	23	6E	42	66	29	6D	109
C3	18	24	6D	43	67	27	6E	110
BC	19	25	6C	44	68	26	6F	111
BA	1A	26	6B	45	69	25	70	112
B9	1B	27	6A	46	70	23	71	113
B6	1C	28	69	47	71	1F	72	114
B5	1D	29	67	48	72	1E	73	115
B4	1E	30	66	49	73	1D	74	116
B3	1F	31	65	4A	74	1B	75	117
B2	20	32	63	4B	75	18	76	118
B1	21	33	5C	4C	76	17	77	119
AE	22	34	5A	4D	77	10	78	120
AD	23	35	59	4E	78	0F	79	121
AC	24	36	56	4F	79	08	7A	122
AB	25	37	55	50	80	04	7B	123
AA	26	38	54	51	81	02	7C	124
A9	27	39	53	52	82	01	7D	125
A7	28	40	52	53	83	00	7E	126
A6	29	41	51	54	84	---	7F	127
A5	2A	42	4E	55	85	---	---	---

Notices

This information was developed for products and services offered in the U. S. A.

IBM may not offer the products, services, or features discussed in this document in other countries. Consult your local IBM representative for information on the products and services currently available in your area. Any reference to an IBM product, program, or service is not intended to state or imply that only that IBM product, program, or service may be used. Any functionally equivalent product, program, or service that does not infringe on any IBM intellectual property right may be used instead. However, it is the user's responsibility to evaluate and verify the operation of any non-IBM product, program, or service.

IBM may have patents or pending patent applications covering subject matter described in this document. The furnishing of this document does not give you any license to these patents. You can send license inquiries, in writing to:

*IBM Director of Licensing
IBM Corporation
North Castle Drive
Armonk, N.Y. 10504-1785 U.S.A.*

The following paragraph does not apply to the United Kingdom or any other country where such provisions are inconsistent with local law:

INTERNATIONAL BUSINESS MACHINES CORPORATION PROVIDES THIS PUBLICATION "AS IS" WITHOUT WARRANTY OF ANY KIND, EITHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF NON-INFRINGEMENT, MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. Some states do not allow disclaimer of express or implied warranties in certain transactions, therefore, this statement may not apply to you.

This information could include technical inaccuracies or typographical errors. Changes are periodically made to the information herein; these changes will be incorporated in new editions of the publication. IBM may make improvements and/or changes in the product(s) and/or the program(s) described in this publication at any time without notice.

Information concerning non-IBM products was obtained from the suppliers of those products, their published announcements or other publicly available sources. IBM has not tested those products and cannot confirm the accuracy of performance, compatibility or any other claims related to non-IBM products. Questions on the capabilities of non-IBM products should be addressed to the suppliers of those products.

IBM may use or distribute any of the information you supply in any way it believes appropriate without incurring any obligation to you.

Trademarks

The following terms are trademarks of the International Business Machines Corporation in the United States, other countries, or both:

IBM
TotalStorage

The following terms are trademarks of the Emulex Corporation in the United States, other countries, or both:

Emulex, Vixel, InSpeed, and FibreSpy

Microsoft, Windows, and Windows NT are trademarks of Microsoft Corporation in the United States, other countries, or both.

UNIX is a registered trademark of The Open Group in the United States and other countries.

Other company, product, or service names may be trademarks or service marks of others.

Electronic emission notices

The following statements apply to this product. The statements for other products intended for use with this product will appear in their accompanying manuals.

Federal Communications Commission (FCC) Class A Statement

Note: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference, in which case the user will be required to correct the interference at his own expense.

IBM is not responsible for any radio or television interference caused by unauthorized changes or modifications to this equipment. Unauthorized changes or modifications could void the user's authority to operate the equipment.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Industry Canada Class A Emission Compliance Statement

This Class A digital apparatus complies with Canadian ICES-003.

Avis de conformité à la réglementation d'Industrie Canada

Cet appareil numérique de la classe A est conforme à la norme NMB-003 du Canada.

European Union (EU) Electromagnetic Compatibility Directive

This product is in conformity with the protection requirements of EU Council Directive 89/336/EEC on the approximation of the laws of the Member States relating to electromagnetic compatibility. IBM cannot accept responsibility for any failure to satisfy the protection requirements resulting from a non-recommended modification of the product, including the fitting of non-IBM option cards.

This product has been tested and found to comply with the limits for Class A Information Technology Equipment according to European Standard EN 55022. The limits for Class A equipment were derived for commercial and industrial environments to provide reasonable protection against interference with licensed communication equipment.

Attention: This is a Class A product. In a domestic environment this product may cause radio interference in which case the user may be required to take adequate measures.

The standards compliance label contains the CE mark, which indicates that this system conforms to the provisions of the following European Council Directives, laws, and standards:

- Electro Magnetic Compatibility (EMC) Directive 89/336/EEC and the Complementary Directives 92/31/EEC and 93/68/EEC.
- Low Voltage Directive (LVD) 73/23/EEC and the Complementary Directive 93/68/EEC.
- EN50082–2/EN55024:1998 (European Immunity Requirements)
 - EN61000–3–2
 - EN61000–3–3/IEC61000–3–3/JEIDA (European and Japanese Harmonics Specification)

Germany Electromagnetic Compatibility Directive

Zulassungsbescheinigung laut dem Deutschen Gesetz über die elektromagnetische Verträglichkeit von Geräten (EMVG) vom 18. September 1998 (bzw. der EMC EG Richtlinie 89/336)

Dieses Gerät ist berechtigt, in Übereinstimmung mit dem Deutschen EMVG das EG-Konformitätszeichen - CE - zu führen.

Verantwortlich für die Konformitätserklärung nach Paragraph 5 des EMVG ist die: IBM Deutschland Informationssysteme GmbH 70548 Stuttgart.

Informationen in Hinsicht EMVG Paragraph 4 Abs. (1) 4:

Das Gerät erfüllt die Schutzanforderungen nach EN 55024 und EN 55022 Klasse A.

EN 55022 Klasse A Geräte müssen mit folgendem Warnhinweis versehen werden: “Warnung: dies ist eine Einrichtung der Klasse A. Diese Einrichtung kann im Wohnbereich Funkstörungen verursachen; in diesem Fall kann vom Betreiber verlangt werden, angemessene Maßnahmen durchzuführen und dafür aufzukommen.”

Anmerkung: Um die Einhaltung des EMVG sicherzustellen, sind die Geräte wie in den IBM Handbüchern angegeben zu installieren und zu betreiben.

Japan VCCI Class A ITE Electronic Emission Statement

この装置は、情報処理装置等電波障害自主規制協議会（VCCI）の基準に基づきクラスA情報技術装置です。この装置を家庭環境で使用すると電波妨害を引き起こすことがあります。この場合には使用者が適切な対策を講ずるよう要求されることがあります。

vcci

Glossary

Table 36. Glossary terms

AL_PA or Arbitrated Loop Physical Address	A one-byte value used to identify a port in an Arbitrated Loop topology. The value of the AL_PA corresponds to bits 7:0 of the 24-bit Native Address Identifier.
Arbitration	The process of selecting one respondent from a group requesting service at the same time.
Close (CLS)	An Arbitrated Loop protocol used to terminate a loop circuit.
CRU	Customer replaceable unit.
Current Fill Word	The fill word that the Loop Port State Machine uses when a fill word is to be transmitted.
Duplex Cable	Two fibers in one cable suitable for duplex transmission.
Fiber Optics	Light transmission through optical fibers for communication or signaling.
Fibre Channel	Fibre Channel is a data transfer interface technology that maps several common transport protocols including IP and SCSI, allowing it to merge high-speed I/O and networking functionality in a single connectivity technology. Fibre channel is an open standard as defined by ANSI and OSI standards and operates over copper and fiber optic cabling at distances of up to 10 kilometers. It is unique in its support of multiple interoperable topologies including point-to-point, arbitrated-loop and switching and it offers several qualities of service for network optimization. With its large packet sizes, Fibre Channel is ideal for storage, video, graphic and mass data transfer applications.
LED	Light-emitting diode. A status indicator on a switch.
Gb/s	Gigabits per second.
Node	An entity with one or more N_Ports or NL_Ports.
Open (OPN)	An Arbitrated Loop protocol used to establish a loop circuit.
Protocol	A data transmission convention which may include timing, control, formatting, error detection with correction and data representation.
SCSI	Small computer system interface. Standard interface for storage modules.
SFP	Small form-factor pluggable transceiver. These transceivers are fully compliant with FC-P1 and MSA standards and occupy less than half the board space of the existing GBIC products.
Topology	The logical and/or physical arrangement of stations on a network. Fibre Channel topologies include point-to-point, Arbitrated Loop, and switched fabric.
Transceiver	A device that converts one form of signaling to another for both transmission and reception. SFPs and GBICs are transceivers.

Index

A

- additional information xvii
- AL_PA Cross References 69
- AL_PA zoning 41, 42
- assistance xviii
- attention notices xiv

B

- Bad Device Recovery policy 33
- Bad Zone Recovery policy 42
- Blocking ARB 23
- Bypass on Clock Delta policy 34
- Bypass on CRC Error policy 34
- Bypass on No Activity policy 33
- Bypass on OS Error policy 33

C

- cascades 43
 - strings 43
 - trees 44
- caution notices xiii
- Change Notification on Insertion policy 32
- Change Notification on Removal policy 32
- change notifications 32
- Clear on Stall policy 33
- CLI
 - commands 65
 - connecting 63
 - frequent tasks 64
 - logging in and out 63
- comments xviii
- configuration files 35, 36
- configuring
 - network interface 13
 - Smart Settings 27
 - switch settings 20
 - Web Manager 15
- custom Smart Settings 29
- customer service xviii

D

- danger notices xi
- date and time settings 24
- desktop installation 6
- device prioritization 48
- diagnostics 34
 - port 53
- displaying
 - event log 51

- ordered sets 55
- port diagnostics 53
- port information 52
- port utilization 52
- switch status 49
- documentation 16
- downloading firmware 35
- downloads xviii

E

- environmental notices
 - fire suppression systems xv
 - product disposal xv
 - product recycling xv
- Ethernet LEDs 7
- event log 51
 - messages 67

F

- Fabric Connection Smart Setting 28
- features, switch 2
- feedback xviii
- files xviii
- fire suppression systems xv
- firmware 35
 - changing versions 36
 - loading 35

G

- glossary 75
- guidelines 6

H

- hard zoning 42
- help xviii

I

- IBM Smart Setting 29
- IBM Smart Settings
 - IBM Linux Initiator 29
 - IBM Linux Stealth Initiator 29
- Initialization Master 38
- Initiator or Target Smart Setting 28
- Initiator with Stealth Smart Setting 28
- InSpeed Technology 3
- installation, switch 5, 6
 - guidelines 6
- installing the switch 5
- introduction 1

J

- joining multiple switches 43

L

- labels xi, xiii
- laser safety xiv
- LEDs
 - 2 Gb/s 8
 - Ethernet 7
 - port 9
 - Port Bypassed 9
 - POST Fault 8
 - Power 8
 - SFP Status 9
 - switch 7
 - Switch Operational 8
 - system 8
- load balancing 46
- loading firmware 35
- logging in and out 63
- logging in to the switch 20

M

- managing the switch 19
- monitoring the switch 49

N

- network interface configuration 13
- network settings 22
- notices 71
 - attention xiv
 - Avis de conformité à la réglementation d'Industrie Canada 72
 - caution xiii
 - danger xi
 - electronic emission 72
 - European Union (EU) Electromagnetic Compatibility Directive 72
 - Federal Communications Commission (FCC) Class A Statement 72
 - Germany Electromagnetic Compatibility Directive 73
 - Industry Canada Class A Emission Compliance Statement 72
 - Japan VCCI Class A ITE Electronic Emission Statement 73

O

- operating conditions 61
- operating speed 22
- ordered sets 55

P

- password 63
 - changing 25
- policies 31, 32, 33, 34

- Bad Device Recovery 33
- Bypass on Clock Delta 34
- Bypass on CRC Error 34
- Bypass on No Activity 33
- Bypass on OS Error 33
- Change Notification on Insertion 32
- Change Notification on Removal 32
- Clear on Stall 33
- Port Test Before Insert (PTBI) 31

port

- diagnostics 53
- hard zoning 42
- information 52
- Smart Settings 28
 - assignments 30
 - change notifications 32
 - creating custom 29
 - diagnostics 34
 - Fabric Connection 28
 - IBM 29
 - IBM Linux Initiator 29
 - IBM Linux Stealth Initiator 29
 - Initiator or Target 28
 - Initiator with Stealth 28
 - port information 31
 - port recovery 33
 - pre-insertion testing 31
 - String Cascade 28
 - Target with Stealth 28
 - Tree Cascade 28
- utilization 52
- port bypass 55
 - conditions and recovery 58
- port information 31
- port LEDs 9
- port reset 55
- Port Test Before Insert (PTBI) policy 31
- ports
 - in multiple zones 40
- powering on the switch 11
- pre-insertion testing 31
- prioritization of devices 48
- product assistance xviii
- product disposal xv
- product recycling xv

R

- rack installation 6
 - guidelines 6
- recycling xv
- references xvii
- restrictions xiv

S

- safety notices xi

- attention xiv
- caution xiii
- danger xi
- laser xiv
- serial interface connection 63
- SFP
 - attaching devices 10
 - compatibility 10
 - installation 10
 - removal 10
- SFPs
 - restrictions xiv
- shipped contents 5
- Smart Settings 27, 28, 59
 - assignments 30
 - change notifications 32
 - creating 29
 - default 59
 - diagnostics 34
 - Fabric Connection 28
 - IBM Linux Initiator 29
 - IBM Linux Stealth Initiator 29
 - IBM Smart Setting 29
 - Initiator or Target 28
 - Initiator with Stealth 28
 - policies 31
 - port information 31
 - port recovery 33
 - pre-insertion testing 31
 - String Cascade 28
 - Target with Stealth 28
 - Tree Cascade 28
- SNMP traps 23
- software updates xviii
- speed, operating 22
- String Cascade Smart Setting 28
- string cascades 43
- switch
 - cascades 43
 - changing the password 25
 - configuration 20
 - configuration files 35, 36
 - date and time settings 24
 - default Smart Settings 59
 - event log 51
 - event log messages 67
 - features 2
 - firmware 35
 - general settings 21
 - hard zoning 42
 - identification 21
 - initial setup 17
 - installation 5, 6
 - LEDs 7

- load balancing 46
- management 13, 19
- monitoring 49
- network settings 22
- operating conditions 61
- ordered sets 55
- package contents 5
- policies 31, 32, 33, 34
- port diagnostics 53
- port information 52
- port utilization 52
- powering on 11
- settings 20
- specifications 61
- speed 22
- status 49
- telnet session 25
- thresholds 26
- trunking 45
- unpacking 5
- version 22
- Web Manager login 20
- zoning 37, 39, 40, 41
- system LEDs 8

T

- Target with Stealth Smart Setting 28
- technical support xviii
- telnet session 25
- temperature 61
- terms
 - see glossary 75
- thresholds 26
- time and date settings 24
- traps 23
- Tree Cascade Smart Setting 28
- tree cascades 44
- troubleshooting 57
- trunking 45

U

- unpacking the switch 5
- updates
 - software xviii
- usage restrictions xiv

V

- version information 22
- viewing
 - event log 51
 - ordered sets 55
 - port diagnostics 53
 - port information 52
 - port utilization 52

switch status 49

W

Web Manager 13

- agent up time 23
- automatic trunking 45
- Bad Zone Recovery 42
- configuration 15
- configuration files 35, 36
- event log 51
- firmware 35
- getting started 13
- hard zoning 42
- initial switch setup 17
- load balancing 46
- loading firmware 35
- network location 22
- network settings 22
- opening a telnet session 25
- ordered sets 55
- overview 15
- password 25
- port diagnostics 53
- port information 52
- port utilization 52
- Smart Settings 27
- SNMP traps 23
- switch identification 21
- switch login 20
- switch speed 22
- switch status 49
- switch thresholds 26
- switch version 22
- time settings 24
- zoning 37, 39, 40, 41

Web sites xvii

Z

Zone Initialization Master 38

zoning 37

- bad zone recovery 42
- hard zoning 42
- Initialization Master 38
- multiple switches 41
- ports in multiple zones 40
- single switch 39
- using AL_PAs 42

Readers' Comments — We'd Like to Hear from You

IBM TotalStorage Storage Switch
2006 Model Installation and User's Guide

Publication No. GC26-7651-00

Overall, how satisfied are you with the information in this book?

	Very Satisfied	Satisfied	Neutral	Dissatisfied	Very Dissatisfied
Overall satisfaction	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

How satisfied are you that the information in this book is:

	Very Satisfied	Satisfied	Neutral	Dissatisfied	Very Dissatisfied
Accurate	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Complete	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Easy to find	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Easy to understand	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Well organized	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Applicable to your tasks	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Please tell us how we can improve this book:

Thank you for your responses. May we contact you? Yes No

When you send comments to IBM, you grant IBM a nonexclusive right to use or distribute your comments in any way it believes appropriate without incurring any obligation to you.

Name

Address

Company or Organization

Phone No.



Fold and Tape

Please do not staple

Fold and Tape




NO POSTAGE
NECESSARY
IF MAILED IN THE
UNITED STATES

BUSINESS REPLY MAIL

FIRST-CLASS MAIL PERMIT NO. 40 ARMONK, NEW YORK

POSTAGE WILL BE PAID BY ADDRESSEE

International Business Machines Corporation
Information Development
Department GZW
9000 South Rita Road
Tucson, AZ 85744-0001



Fold and Tape

Please do not staple

Fold and Tape

